

My Alerts

07 Jun 2025 06:58  Left ventricular pacing lead impedance out of range.

For Technical Support contact 1-800-CARDIAC (Americas) or your local Boston Scientific Representative.

Events Since Last Reset (14 Mar 2024)

09 Jan 2025 20:26 ATR at 248 min⁻¹, Avg V Rate in ATR: 70 min⁻¹

09 Jan 2025 19:23 ATR at 182 min⁻¹, Avg V Rate in ATR: 70 min⁻¹


See last page for full list of Events Since Last Reset.

Battery OK

Approximate time to explant: 8 months from 08 Jun 2025

Magnet Rate 90 min⁻¹

One Year Remaining

Explant 


See last page for additional battery information.


Leads	Implant (N/R N/R N/R)	Most Recent In-Office Measurement (23 Apr 2025)	Most Recent Daily Measurement (07 Jun 2025)
 An automatic safety switch from bipolar to unipolar occurred on 07 Jun 2025 due to an LV Pace Impedance measurement of >3000 Ω.			
 Atrial			
Intrinsic Amplitude	N/R	N/R	N/R
Pace Impedance	N/R	453 Ω	473 Ω
Pace Threshold	N/R	0.1 V @ 0.4 ms	N/R
 Right Ventricular			
Intrinsic Amplitude	N/R	N/R	N/R
Pace Impedance	N/R	345 Ω	354 Ω
Pace Threshold	N/R	1.3 V @ 0.4 ms	N/R
 Left Ventricular			
Intrinsic Amplitude	N/R	N/R	N/R
Pace Impedance	N/R	323 Ω	 >3000 Ω
Pace Threshold	N/R	1.5 V @ 0.4 ms	N/R


Settings

Ventricular Tachy			
Ventricular Tachy EGM Storage			On
Detection Rate			160 min ⁻¹ (375 ms)
Brady/CRT		Pacing Output	
Mode	VVIR	 Right Ventricular	4.0 V @ 0.4 ms
Lower Rate Limit	60 min ⁻¹	 Left Ventricular	4.0 V @ 0.4 ms
Maximum Sensor Rate	130 min ⁻¹	Sensitivity	
RV-Refractory (RVRP)	230 - 250 ms	 Atrial	Fixed 0.75 mV
LV-Refractory (LVRP)	250 ms	 Right Ventricular	Fixed 2.5 mV
Ventricular Pacing Chamber	BiV	 Left Ventricular	Fixed 2.5 mV
LV Offset	0 ms	Leads Configuration (Pace/Sense)	
		 Atrial	-/Off
		 Right Ventricular	Bipolar
		 Left Ventricular	 LVtip>>Can
		Rate Adaptive Pacing	
		Minute Ventilation	 Disabled
		Accelerometer	On

Trend Graphs

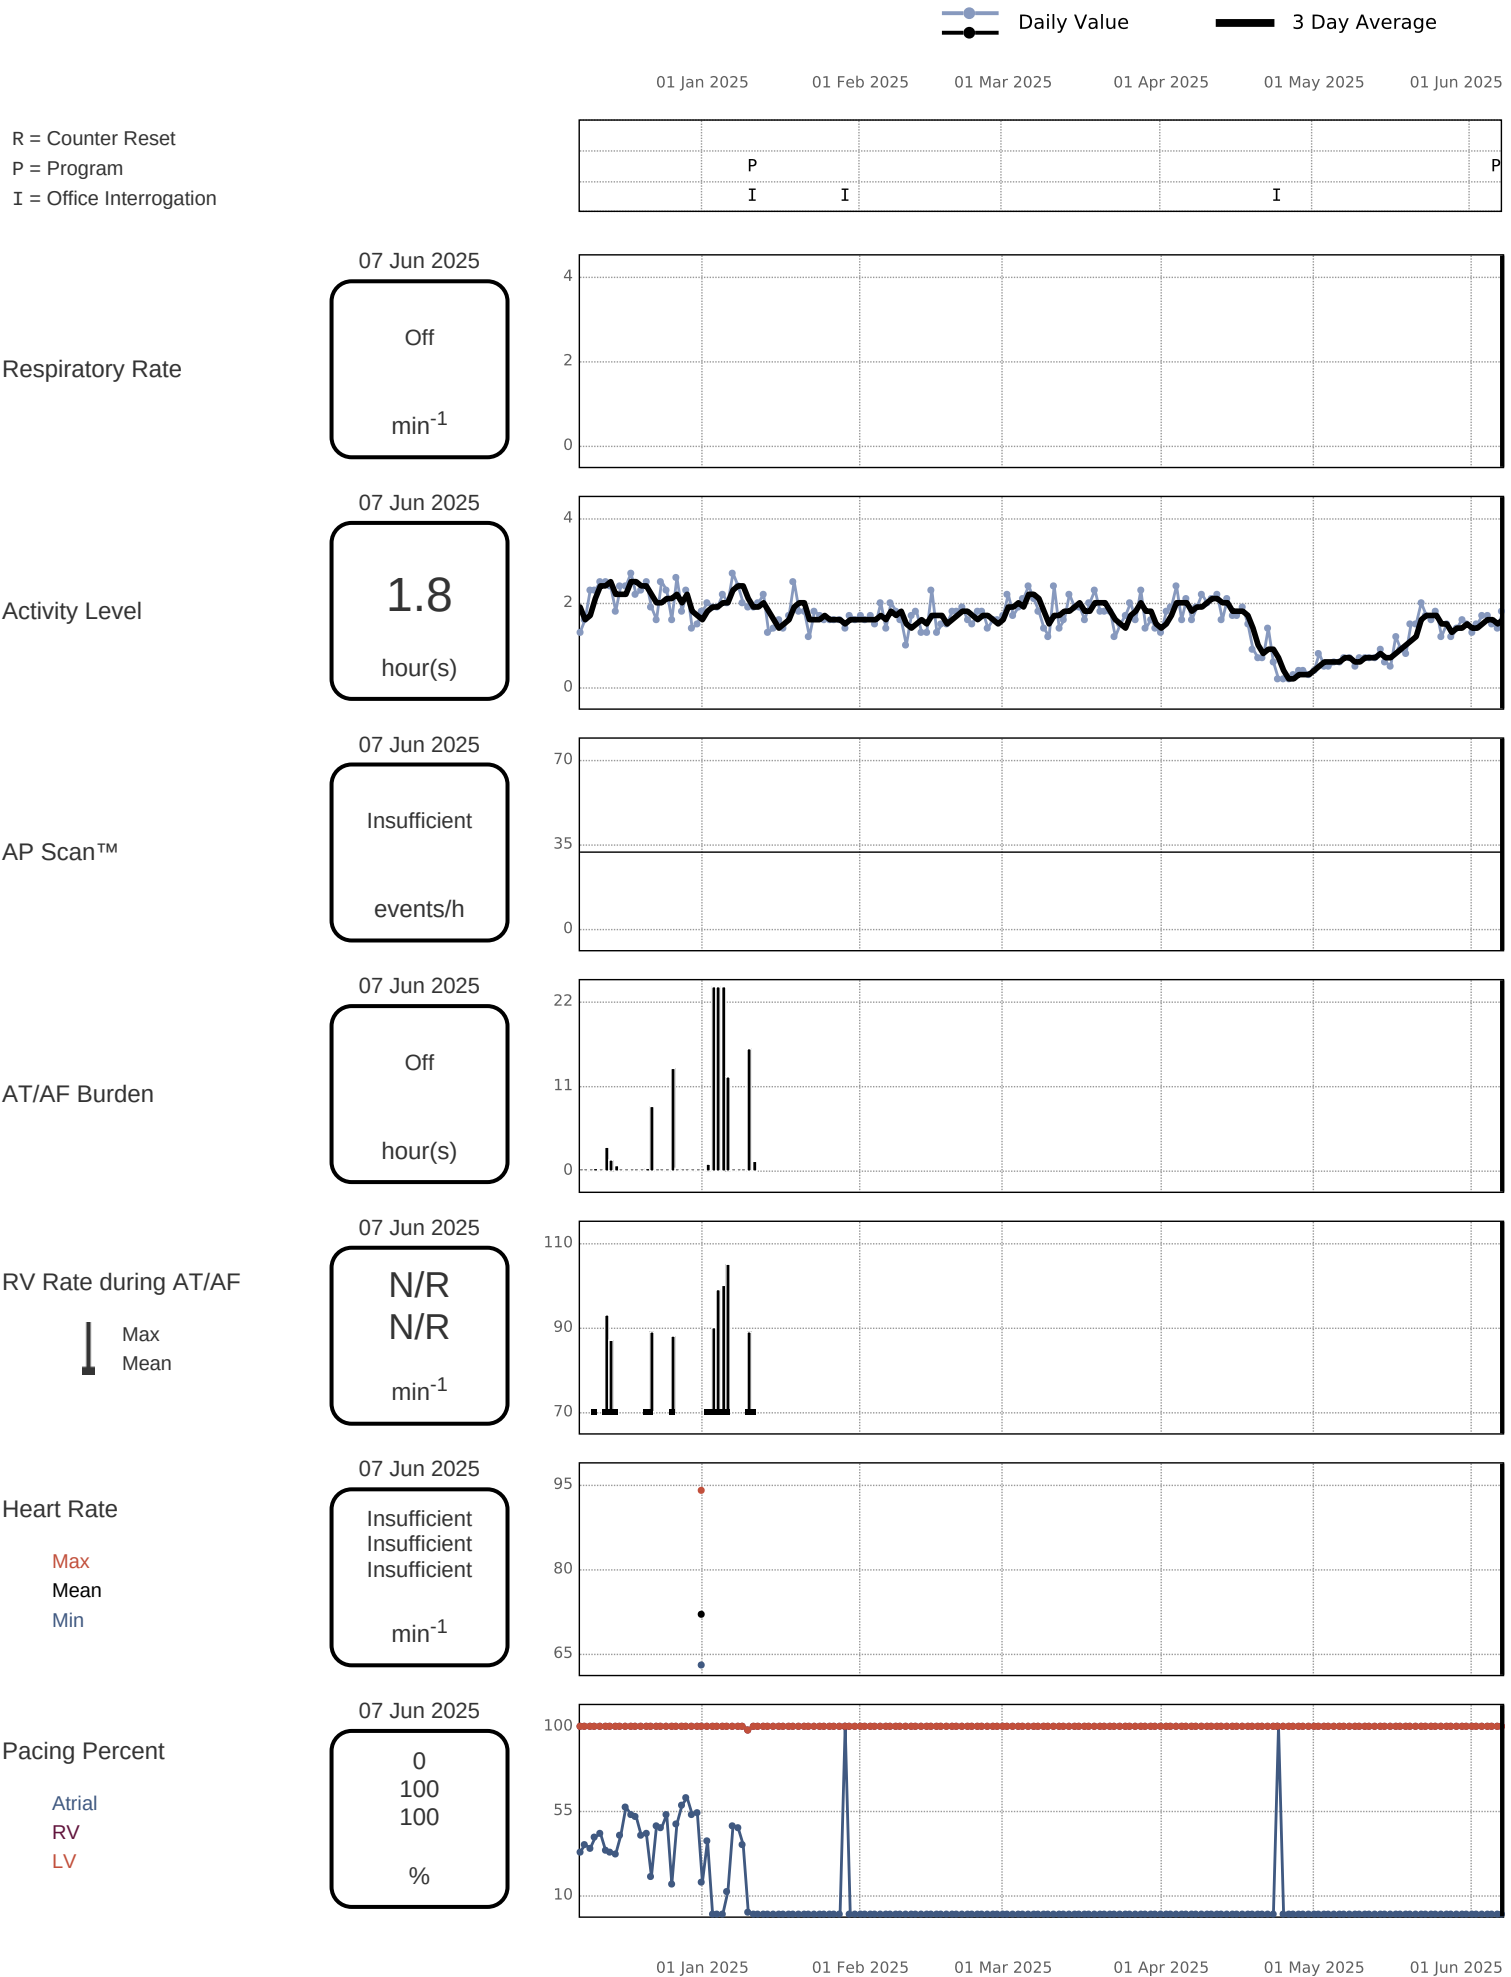

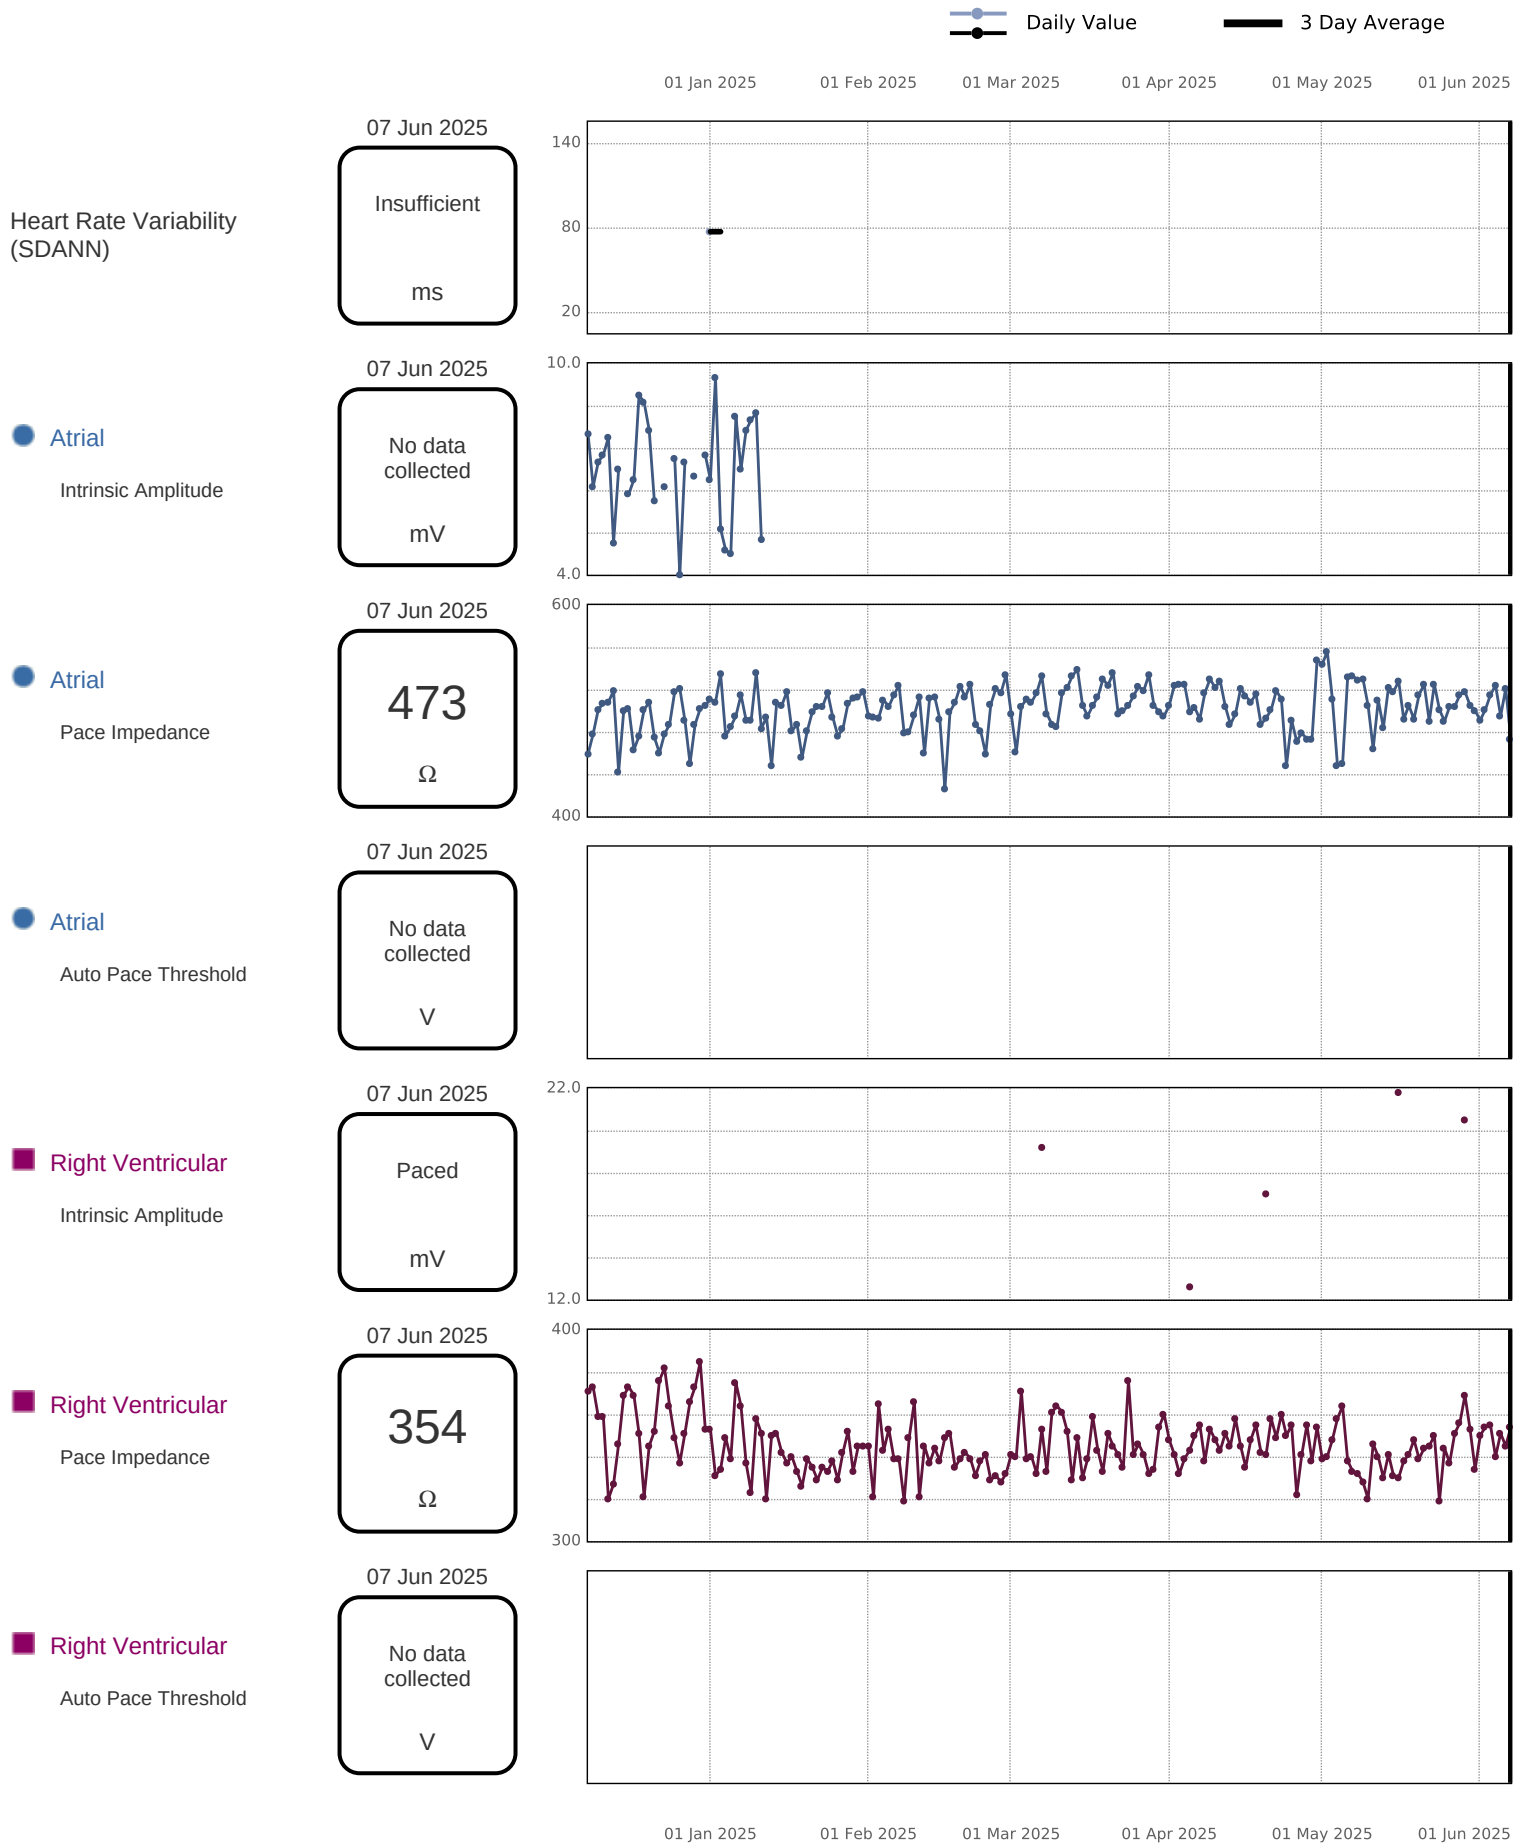

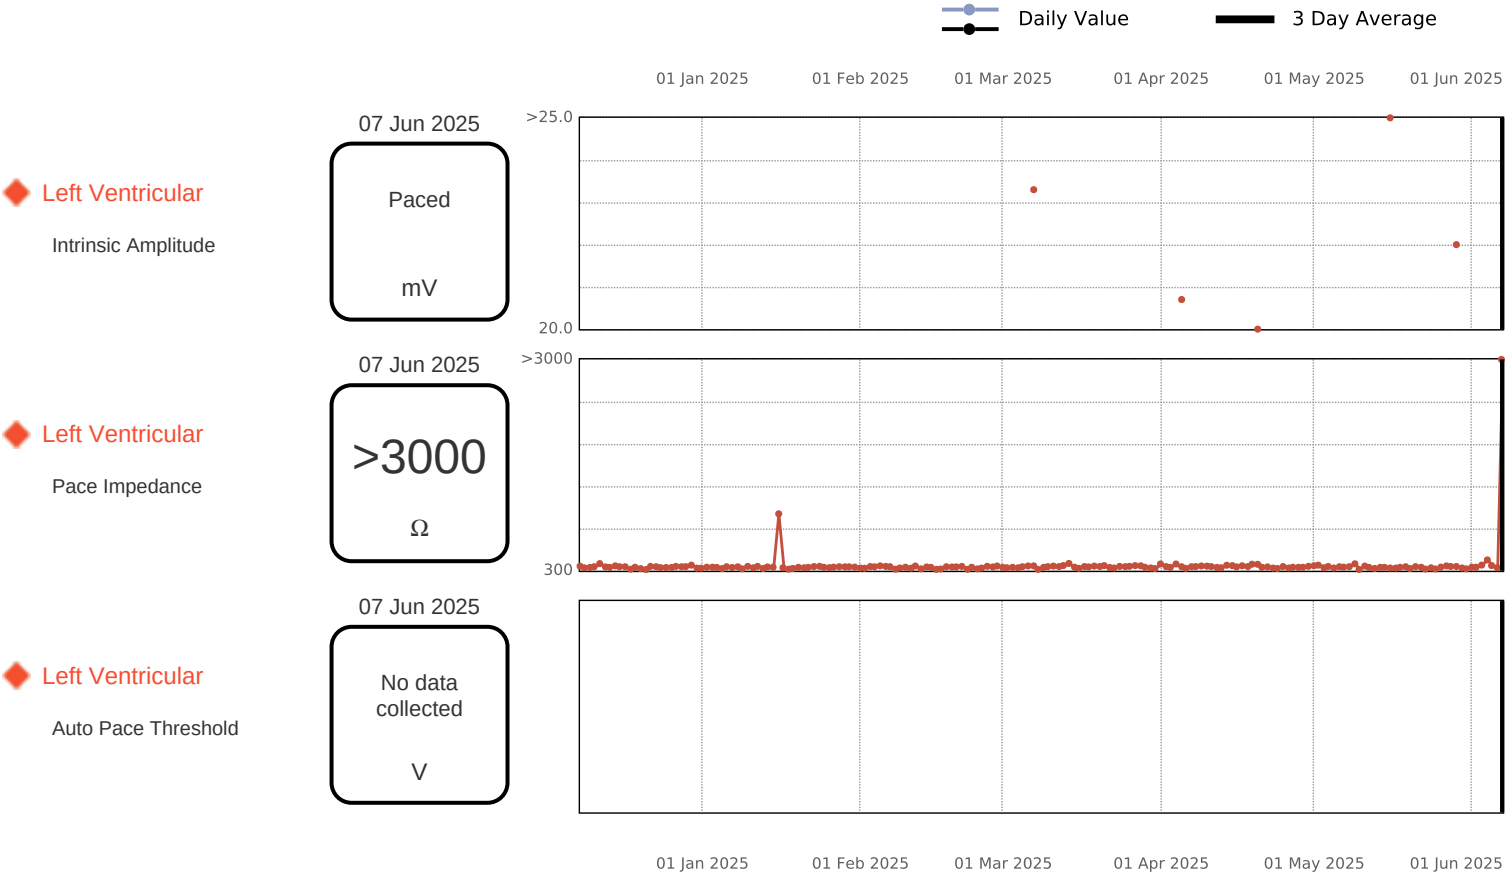

Ventricular Tachy Counters	Since Last Reset 14 Mar 2024	Device Totals
----------------------------	---------------------------------	---------------

Ventricular Episode Counters		
Total Episodes	0	0
VT Episodes (V>A)	0	0
SVT Episodes (V<=A)	0	0
NonsustainedV Episodes	0	0

Brady/CRT Counters	Reset Before Last 1213 day(s) 17 Nov 2020 to 14 Mar 2024	Since Last Reset 450 day(s) 14 Mar 2024 to 08 Jun 2025
--------------------	--	--


Counters		
% A Paced	13	49
% RV Paced	100	100
% LV Paced	100	100
Intrinsic Promotion		
Rate Hysteresis		
% Successful	0	0
Atrial Arrhythmia		
% AT/AF (One Year of Data)	N/R	5
Total Time in AT/AF (days) (One Year of Data)	N/R	19.4
Episodes by Duration		
< 1 minute	26	48
1 min - < 1 hr	29	42
1 hr - < 24 hr	33	34
24 hr - < 48 hr	4	3
> 48 hr	4	2
Total PACs	361282	224468
Ventricular Counters		
Total PVCs	172695	7523
Three or More PVCs	15	0

AT/AF Overview: Since Last Reset (14 Mar 2024 to 08 Jun 2025)		
AT/AF (One Year of Data): 5 %	AT/AF Events: 129	
Total Time in AT/AF (days) (One Year of Data): 19.4		
Most Recent: 09 Jan 2025 20:26	Avg V Rate: 70 min ⁻¹	Duration: 15:20:43 hh:mm:ss
Longest: 31 Aug 2024 19:24	Avg V Rate: 70 min ⁻¹	Duration: >48 Hours
Fastest RVS Rate: 21 Sep 2024 13:31	Max V Rate: 117 min ⁻¹	Duration: 11:34:15 hh:mm:ss
AT/AF Overview: Reset Before Last (17 Nov 2020 to 14 Mar 2024)		
Longest: 28 Apr 2023 13:50	Avg V Rate: 71 min ⁻¹	Duration: >48 Hours
Fastest RVS Rate: 28 Apr 2023 13:50	Max V Rate: 149 min ⁻¹	Duration: >48 Hours


Histograms




Atrial Activity

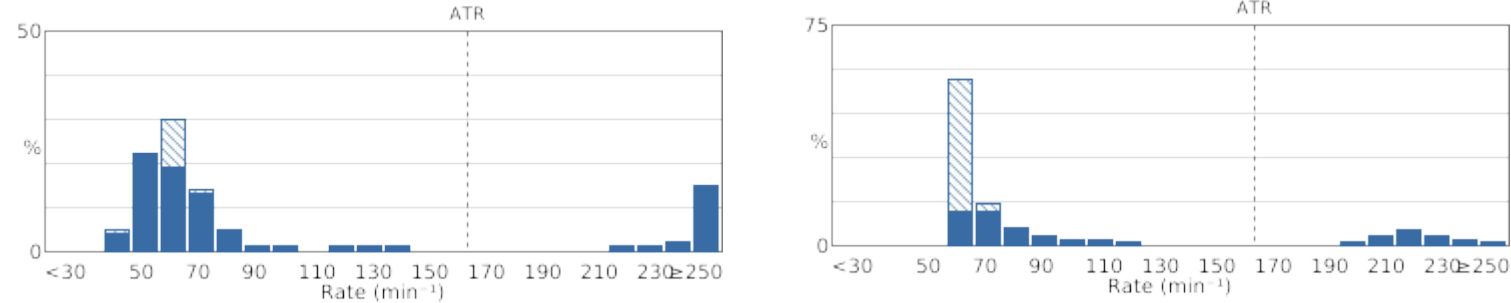


Ventricular Activity

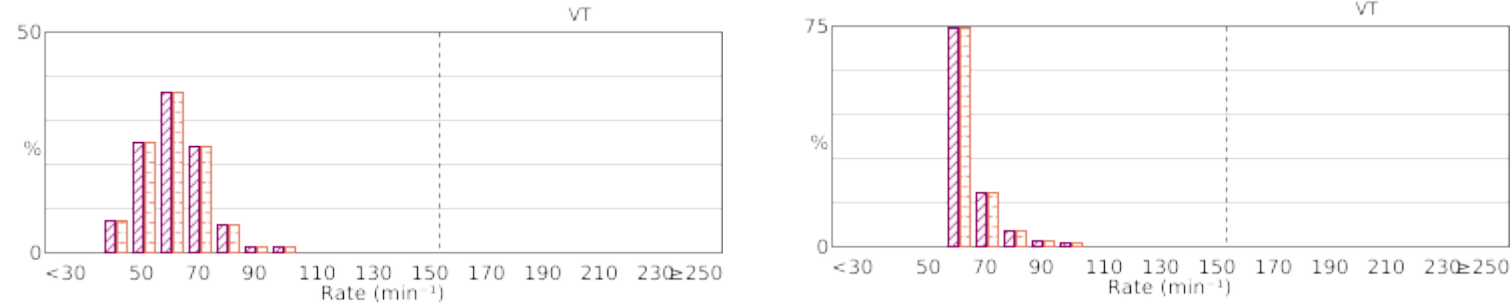


Ventricular Response to Atrial Pace

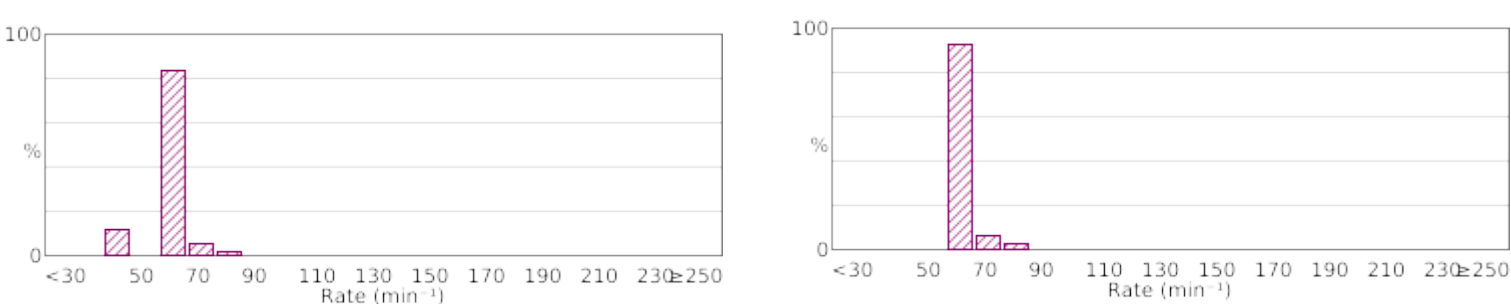

Ventricular Response to Atrial Sense

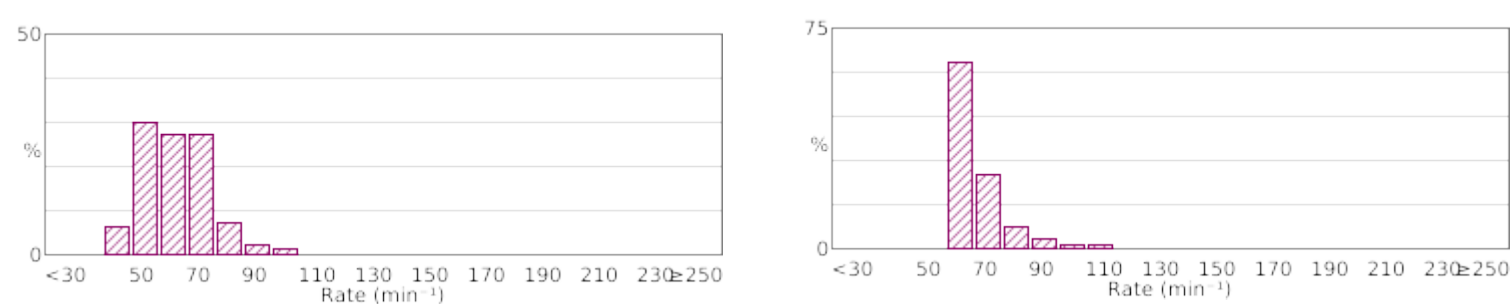

RV Rate during AT/AF

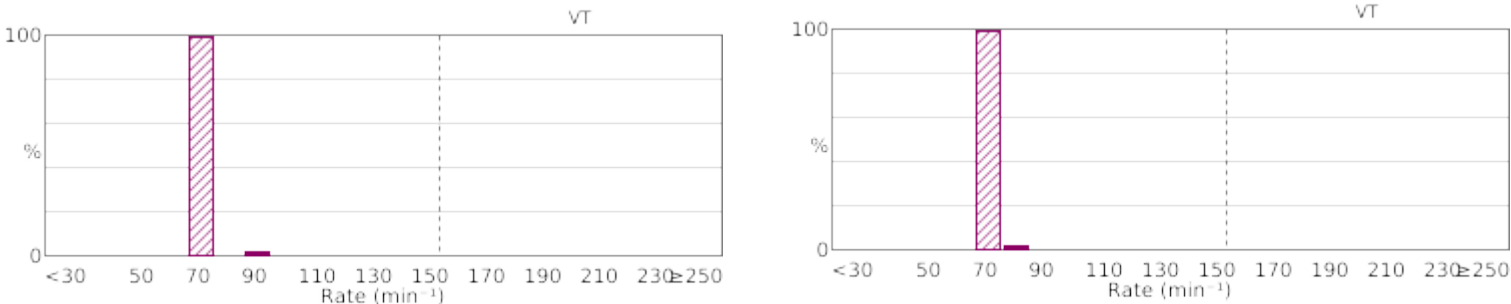

Reset Before Last 1213 day(s) 17 Nov 2020 to 14 Mar 2024			Since Last Reset 450 day(s) 14 Mar 2024 to 08 Jun 2025	
Atrial				
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	0	177	0	76
30-39	4	7.5K	22	724
40-49	1.9M	5.6M	13	589
50-59	330	27.6M	277	672
60-69	14.1M	24.2M	14.8M	3.8M
70-79	838.3K	16.2M	1.0M	3.5M
80-89	198.8K	6.2M	284.6K	1.7M
90-99	36.9K	1.6M	42.8K	914.3K
100-109	517	708.9K	421	647.4K
110-119	23	464.6K	22	636.1K
120-129	0	1.6M	0	195.8K
130-139	0	1.3M	0	13.3K
140-149	0	1.5M	0	4.5K
150-159	0	91.2K	0	2.4K
160-169	0	51.6K	0	2.7K
170-179	0	48.5K	0	4.7K
180-189	0	40.3K	0	15.4K
190-199	0	40.3K	0	76.6K
200-209	0	155.4K	0	490.3K
210-219	0	344.2K	0	931.2K
220-229	0	640.4K	0	1.7M
230-239	0	686.3K	0	995.8K
240-249	0	2.0M	0	794.0K
>=250	7	19.7M	0	330.5K

Right Ventricular	Reset Before Last 1213 day(s) 17 Nov 2020 to 14 Mar 2024		Since Last Reset 450 day(s) 14 Mar 2024 to 08 Jun 2025	
	Rate (min ⁻¹)	Paced	Sensed	Paced
0-29	0	0	0	0
30-39	0	0	11	1
40-49	7.5M	177	6	0
50-59	27.7M	806	526	0
60-69	38.9M	1.2K	31.1M	352
70-79	25.8M	5.5K	7.4M	8.4K
80-89	6.4M	44.3K	2.0M	29.9K
90-99	1.5M	125.0K	818.9K	10.8K
100-109	609.6K	117.5K	342.8K	539
110-119	267.1K	19.8K	145.1K	819
120-129	57.9K	2.7K	9.3K	111
130-139	17.4K	599	2.0K	34
140-149	0	231	0	33
150-159	0	117	0	24
160-169	0	84	0	4
170-179	0	30	0	4
180-189	0	12	0	1
190-199	0	8	0	0
200-209	0	4	0	0
210-219	0	6	0	2
220-229	0	1	0	0
230-239	0	2	0	0
240-249	0	0	0	0
>=250	0	0	0	0


Reset Before Last 1213 day(s)			Since Last Reset 450 day(s)	
Left Ventricular 17 Nov 2020 to 14 Mar 2024			14 Mar 2024 to 08 Jun 2025	
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	21	4	1	0
30-39	25	1	29	2
40-49	7.5M	172	58	0
50-59	27.7M	901	7.9K	83
60-69	38.9M	1.3K	31.1M	338
70-79	25.8M	8.4K	7.4M	5.3K
80-89	6.4M	33.5K	2.0M	24.7K
90-99	1.6M	47.2K	811.6K	26.3K
100-109	631.5K	62.4K	342.7K	2.1K
110-119	265.8K	41.4K	145.1K	838
120-129	58.8K	5.2K	9.3K	210
130-139	17.4K	758	2.0K	70
140-149	26	352	31	74
150-159	0	162	2	37
160-169	0	122	0	21
170-179	0	32	0	25
180-189	0	26	0	31
190-199	0	10	0	26
200-209	0	4	0	27
210-219	0	5	0	27
220-229	0	1	0	25
230-239	0	4	0	23
240-249	0	0	0	0
>=250	0	0	0	0

Reset Before Last 1213 day(s)			Since Last Reset 450 day(s)	
RV Rate during AT/AF 17 Nov 2020 to 14 Mar 2024			14 Mar 2024 to 08 Jun 2025	
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	0	0	0	0
30-39	0	0	0	0
40-49	0	0	0	0
50-59	1	0	0	0
60-69	41	0	0	0
70-79	8.8M	3.2K	2.3M	4.9K
80-89	47	28.6K	78	13.1K
90-99	14	59.8K	10	1.0K
100-109	2	22.8K	0	23
110-119	0	4.4K	0	44
120-129	0	274	0	12
130-139	0	125	0	1
140-149	0	27	0	3
150-159	0	5	0	3
160-169	0	3	0	0
170-179	0	1	0	0
180-189	0	0	0	0
190-199	0	0	0	0
200-209	0	0	0	0
210-219	0	0	0	0
220-229	0	0	0	0
230-239	0	0	0	0
240-249	0	0	0	0
>=250	0	0	0	0

Heart Rate Variability


Last measured for 24-hr period ending 01 Jan 2025 11:20

% of Time Used	71
Footprint	32 %
SDANN	77 ms
Mode	DDDR
Sensed AV Delay	120 ms
Ventricular Pacing Chamber	BiV
LV Offset	0 ms

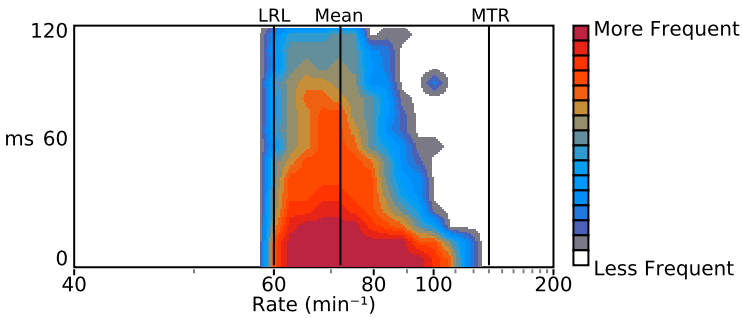



Reference: 24-hr period ending 08 May 2019 10:38



% of Time Used	80
Footprint	22 %
SDANN	34 ms
Mode	DDD
Sensed AV Delay	110 ms
Ventricular Pacing Chamber	BiV
LV Offset	0 ms

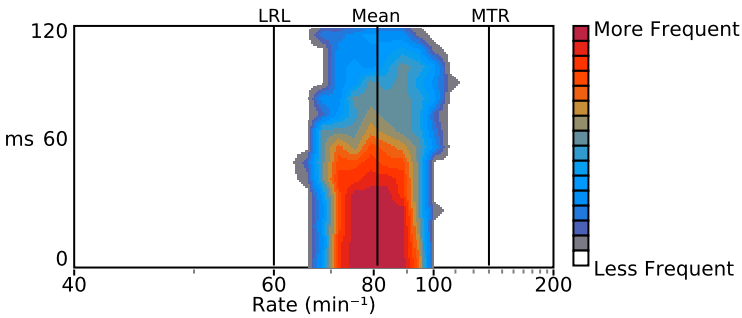


Presenting EGM (08 Jun 2025)

EGM displayed at 25mm per second

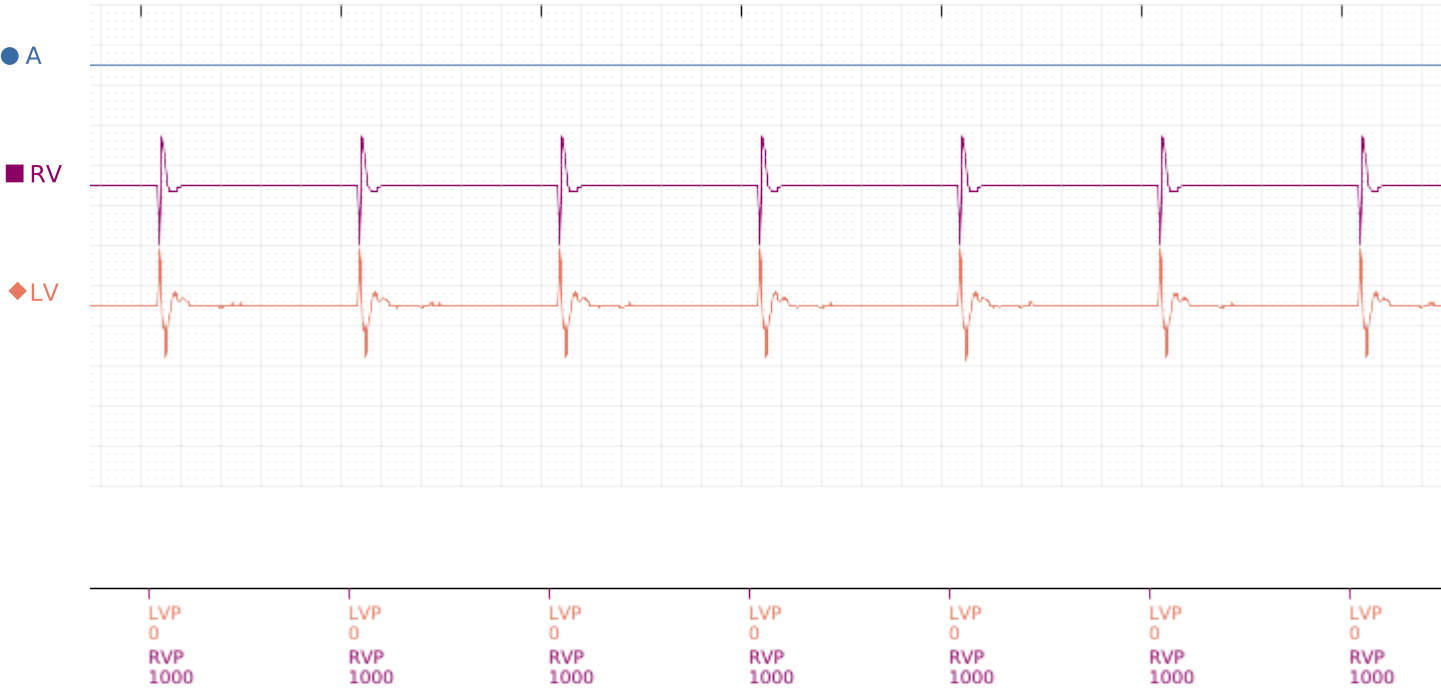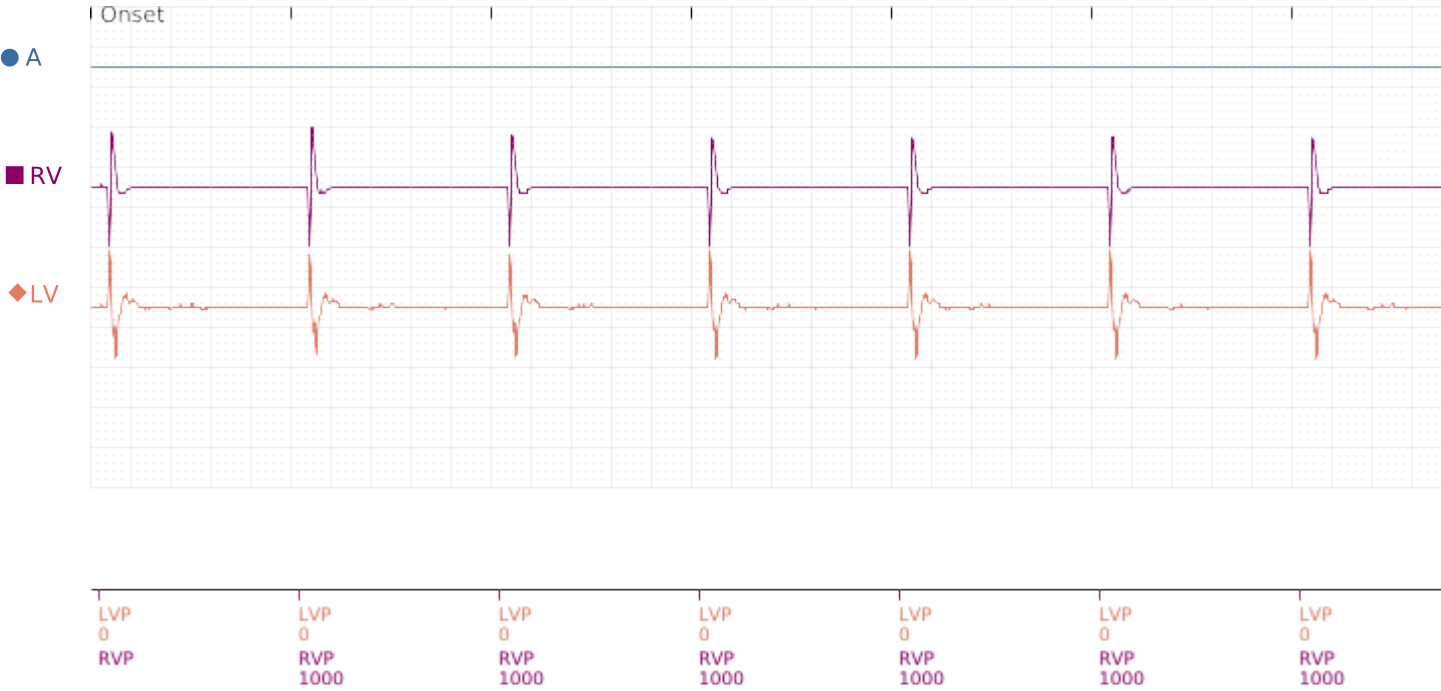

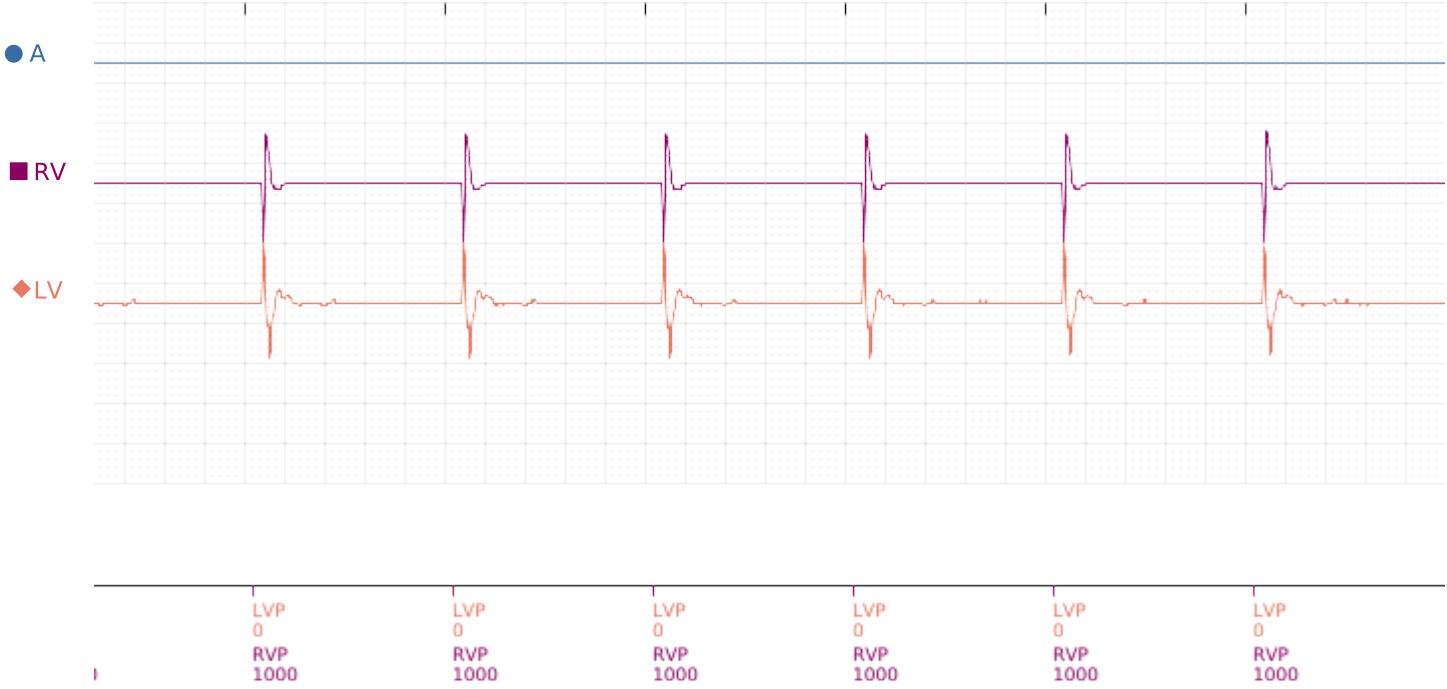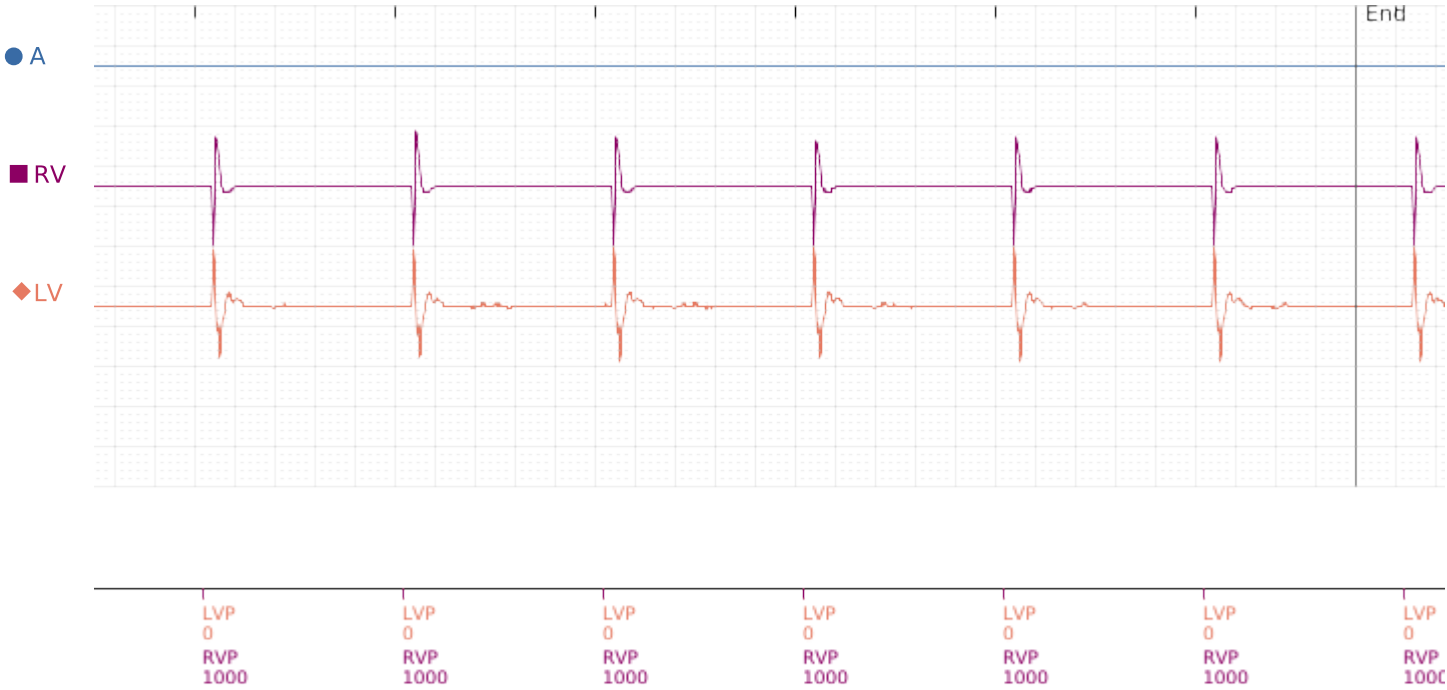

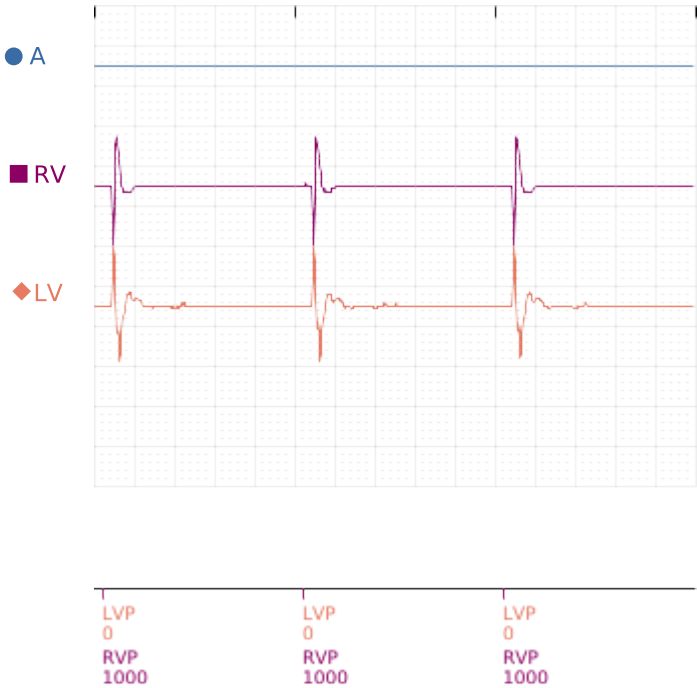

All Events Since Last Reset (14 Mar 2024)

09 Jan 2025 20:26	ATR at 248 min ⁻¹ , Avg V Rate in ATR: 70 min ⁻¹
09 Jan 2025 19:23	ATR at 182 min ⁻¹ , Avg V Rate in ATR: 70 min ⁻¹
02 Jan 2025 10:25	ATR at 222 min ⁻¹ , Avg V Rate in ATR: 70 min ⁻¹
25 Dec 2024 11:25	ATR at 174 min ⁻¹ , Avg V Rate in ATR: 70 min ⁻¹
21 Dec 2024 17:44	ATR at 214 min ⁻¹ , Avg V Rate in ATR: 70 min ⁻¹
21 Dec 2024 17:26	ATR at 223 min ⁻¹ , Avg V Rate in ATR: 70 min ⁻¹
21 Dec 2024 17:04	ATR at 178 min ⁻¹ , Avg V Rate in ATR: 70 min ⁻¹
20 Dec 2024 20:20	ATR at 297 min ⁻¹ , Avg V Rate in ATR: 71 min ⁻¹
20 Dec 2024 19:53	ATR at 229 min ⁻¹ , Avg V Rate in ATR: 70 min ⁻¹
14 Dec 2024 11:44	ATR at 173 min ⁻¹ , Avg V Rate in ATR: 70 min ⁻¹
15 Oct 2024 09:22	PMT at 130 min ⁻¹
15 Oct 2024 09:20	PMT at 130 min ⁻¹
15 Oct 2024 09:19	PMT at 130 min ⁻¹
Total Events: 129 ATR	

Battery (Continued)

Time Since Implant	74 months
Charge Remaining	0.32 ampere-hours
Power Consumption	69 μW
(Measured with programmed parameters)	
This device is using 129% of the power it would use at the following parameters:	
● A	15% pacing, 70 min ⁻¹ , 2.5 V, 0.4 ms, 500 Ω
■ RV	100% pacing, 70 min ⁻¹ , 2.5 V, 0.4 ms, 500 Ω
◆ LV	100% pacing, 70 min ⁻¹ , 3.5 V, 0.4 ms, 700 Ω