

My Alerts

28 May 2022 13:23  Nonsustained ventricular arrhythmia episode(s).

For Technical Support contact 1-800-CARDIAC (Americas) or your local Boston Scientific Representative.

Events Since Last Reset (03 May 2022)

28 May 2022 13:23 NonSustV at 175 min⁻¹

28 May 2022 08:26 RA Auto


See last page for full list of Events Since Last Reset.

Battery

Approximate time to explant: 1 year from 29 May 2022

Magnet Rate 100 min⁻¹

One Year Remaining

Explant 

See last page for additional battery information.

Leads	Implant (N/R N/R N/R)	Most Recent In-Office Measurement (03 May 2022)	Most Recent Daily Measurement (28 May 2022)
Atrial			
Intrinsic Amplitude	N/R	6.0 mV	3.6 mV
Pace Impedance	N/R	547 Ω	522 Ω
Pace Threshold	N/R	Auto 0.4 V @ 0.4 ms	0.4 V @ 0.4 ms
Right Ventricular			
Intrinsic Amplitude	N/R	22.2 mV	N/R
Pace Impedance	N/R	657 Ω	615 Ω
Pace Threshold	N/R	Auto 0.7 V @ 0.4 ms	0.8 V @ 0.4 ms
Left Ventricular			
Intrinsic Amplitude	N/R	4.4 mV	N/R
Pace Impedance	N/R	676 Ω	1625 Ω
Pace Threshold	N/R	1.6 V @ 0.8 ms	


Settings

Ventricular Tachy			On		
Ventricular Tachy EGM Storage			160 min ⁻¹ (375 ms)		
Detection Rate					
Atrial Tachy			Pacing Output		
ATR Mode Switch	170 min ⁻¹	DDI	Atrial	Trend 2.0 V @ 0.4 ms	
Brady/CRT			Right Ventricular	Trend 2.0 V @ 0.4 ms	
Mode		DDD	Left Ventricular	2.5 V @ 0.8 ms	
Lower Rate Limit		50 min ⁻¹	Sensitivity		
Maximum Tracking Rate		120 min ⁻¹	Atrial	Fixed 0.75 mV	
Paced AV Delay		100 - 150 ms	Right Ventricular	Fixed 2.5 mV	
Sensed AV Delay		80 - 120 ms	Left Ventricular	Fixed 2.5 mV	
A-Refractory (PVARP)		240 - 280 ms	Leads Configuration (Pace/Sense)		
RV-Refractory (RVRP)		230 - 250 ms	Atrial	Bipolar	
LV-Refractory (LVRP)		250 ms	Right Ventricular	Bipolar	
Ventricular Pacing Chamber		BiV	Left Ventricular	LVTip1>>LVRing2	
LV Offset		0 ms	Rate Adaptive Pacing		
			Minute Ventilation	Passive	
			Accelerometer	Passive	



 Daily Value
  3 Day Average

					R
					P
					I


13
min⁻¹

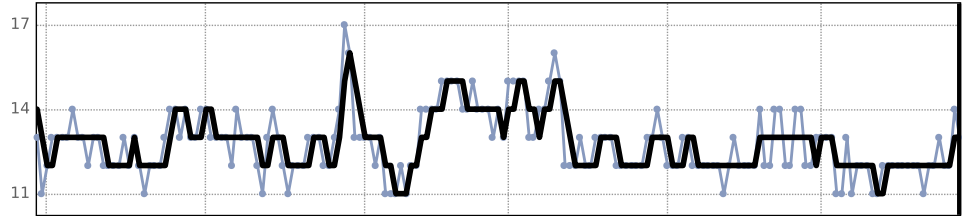


1.3
hour(s)

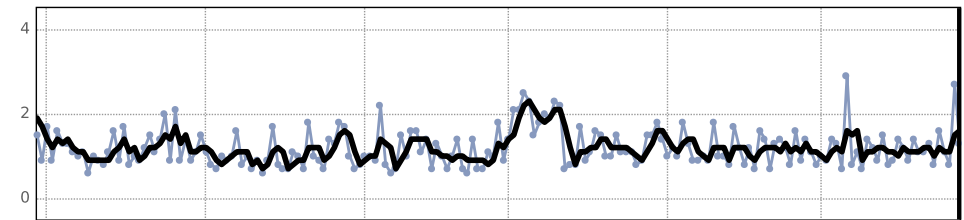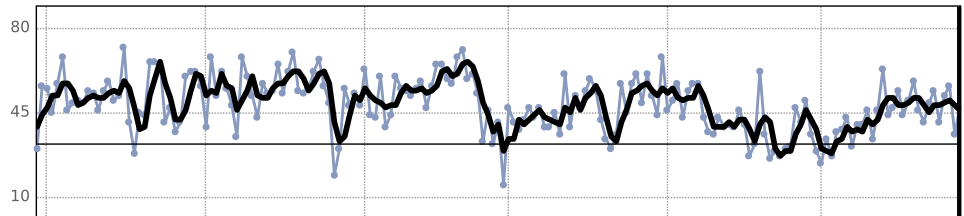47
events/h


0.0
hour(s)

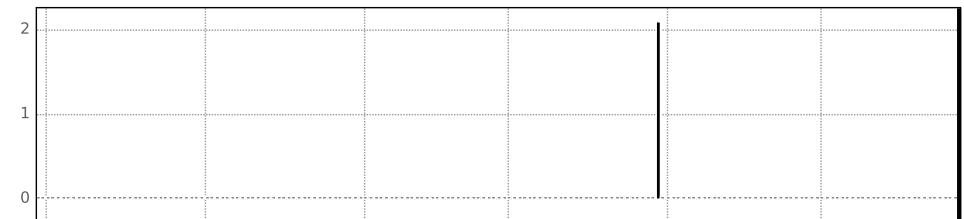


N/R
N/R
min⁻¹

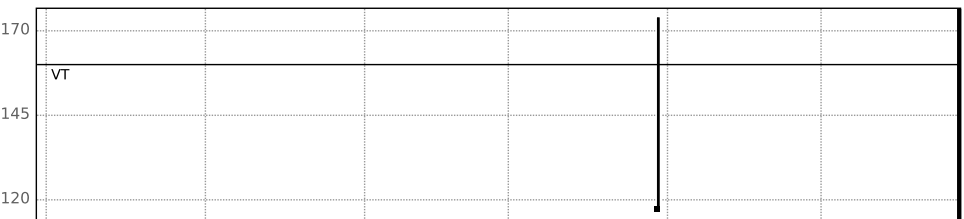


87
76
66
min⁻¹

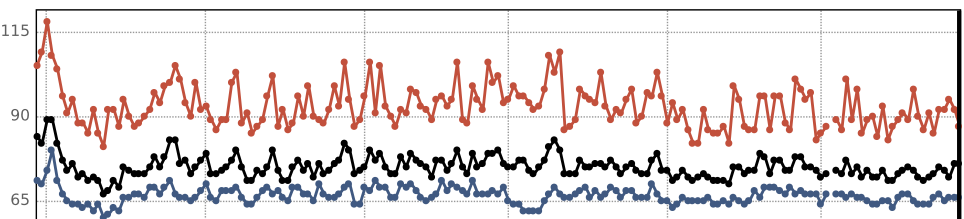


0
100
100
%

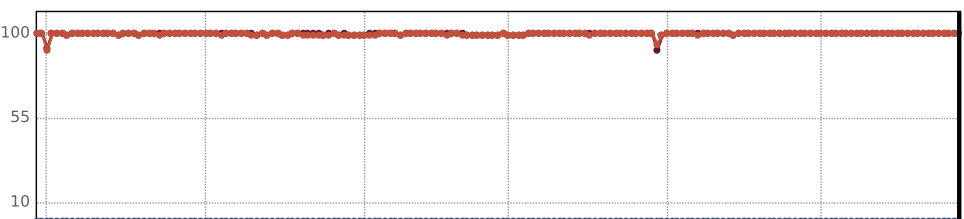

01 Dec 2021	01 Jan 2022	01 Feb 2022	01 Mar 2022	01 Apr 2022	01 May 2022
-------------	-------------	-------------	-------------	-------------	-------------

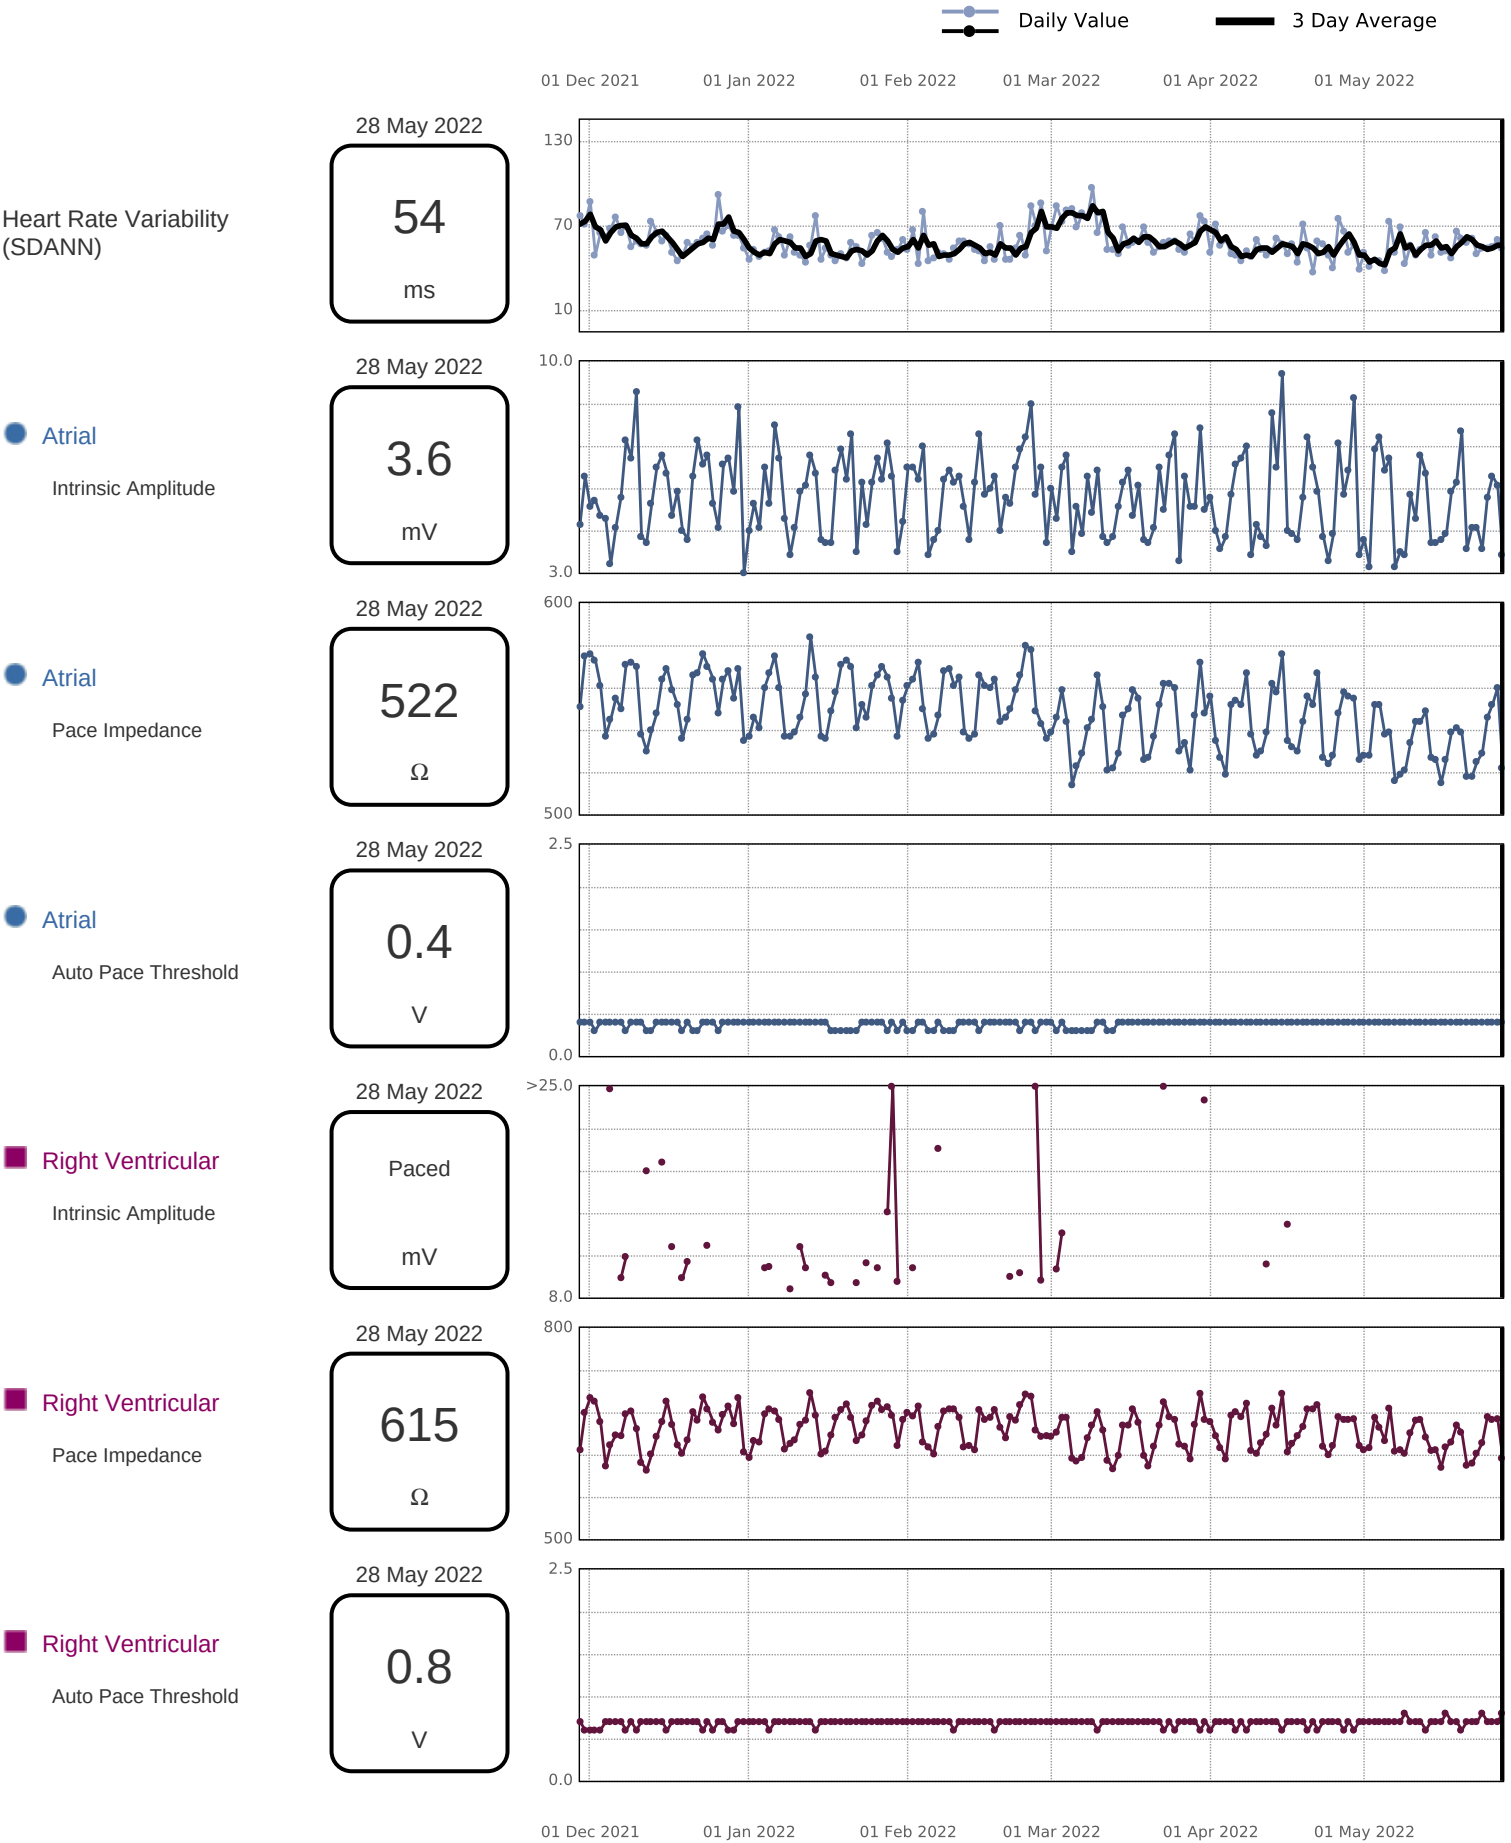

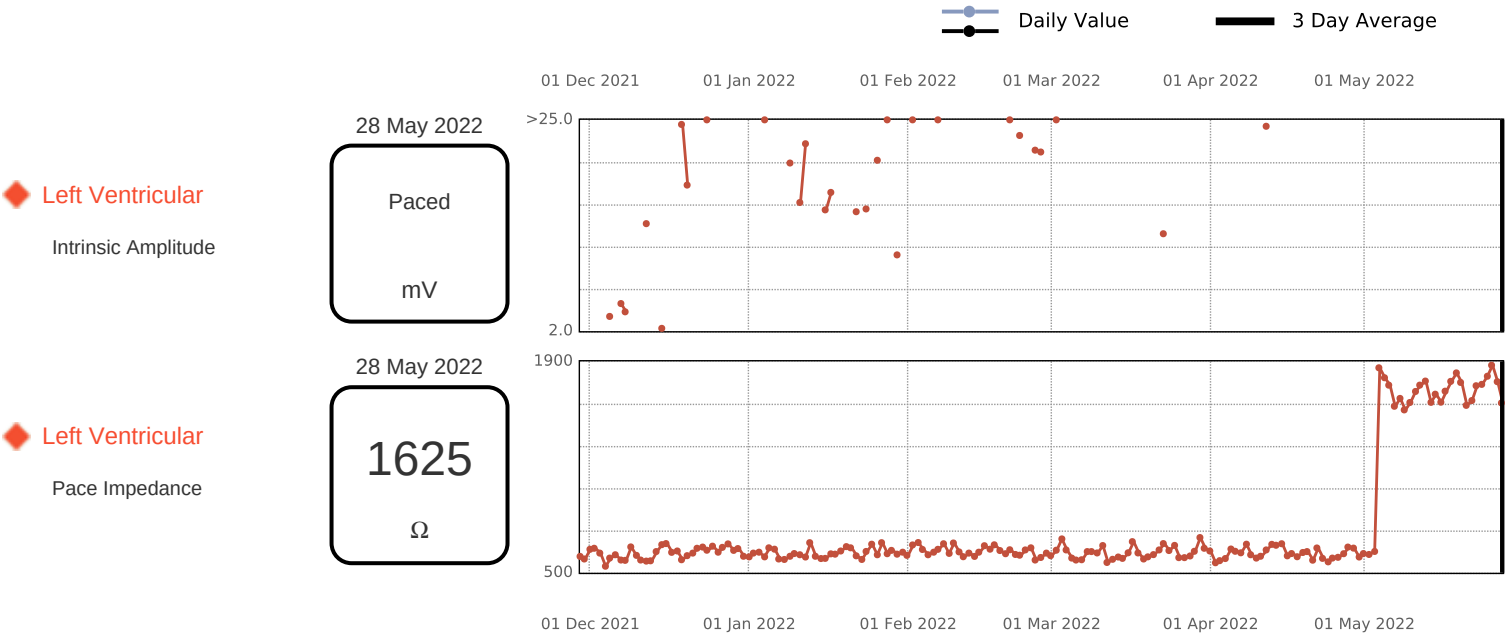

Ventricular Tachy Counters	Since Last Reset 03 May 2022	Device Totals
----------------------------	---------------------------------	---------------

Ventricular Episode Counters		
Total Episodes	1	5
VT Episodes (V>A)	0	0
SVT Episodes (V<=A)	0	0
⚠ NonsustainedV Episodes	1	5

Brady/CRT Counters	Reset Before Last 1042 day(s)	Since Last Reset
	26 Jun 2019 to 03 May 2022	25 day(s)

Counters		
% A Paced	0	0
% RV Paced	100	100
% LV Paced	99	100
Intrinsic Promotion		
Rate Hysteresis		
% Successful	0	0
Atrial Arrhythmia		
% AT/AF (One Year of Data)	<1	0
Total Time in AT/AF (hr) (One Year of Data)	2.1	0.0
Episodes by Duration		
< 1 minute	5	0
1 min - < 1 hr	1	0
1 hr - < 24 hr	1	0
24 hr - < 48 hr	0	0
> 48 hr	0	0
Total PACs	12491	247
Ventricular Counters		
Total PVCs	361919	1036
Three or More PVCs	19	2






AT/AF Overview: Since Last Reset (03 May 2022 to 29 May 2022)

AT/AF (One Year of Data): 0 %	AT/AF Events: 0
Total Time in AT/AF (hr) (One Year of Data): 0.0	
There are no ATR events to display.	

AT/AF Overview: Reset Before Last (26 Jun 2019 to 03 May 2022)

Longest: 29 Mar 2022 23:43	Avg V Rate: 117 min ⁻¹	Duration: 02:05:24 hh:mm:ss
Fastest RVS Rate: 29 Mar 2022 23:43	Max V Rate: 174 min ⁻¹	Duration: 02:05:24 hh:mm:ss

Histograms

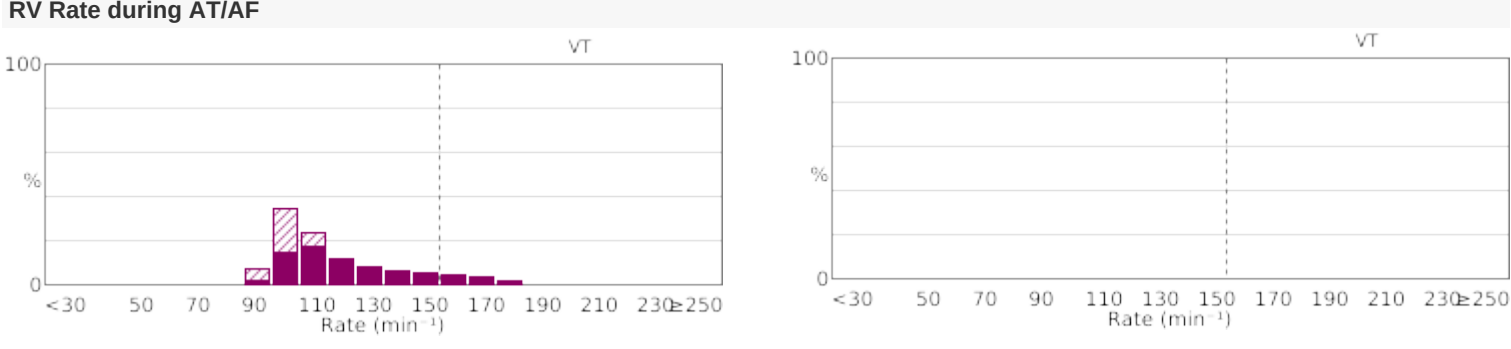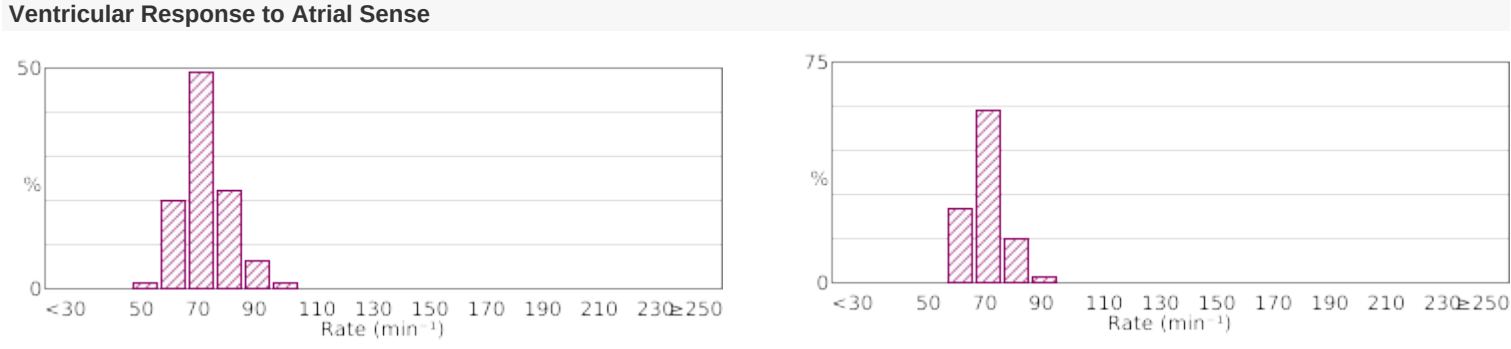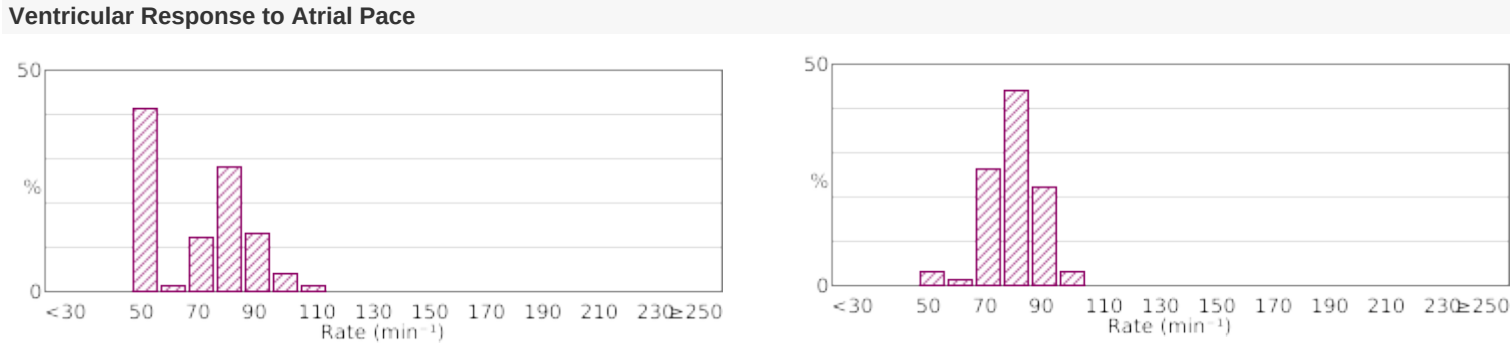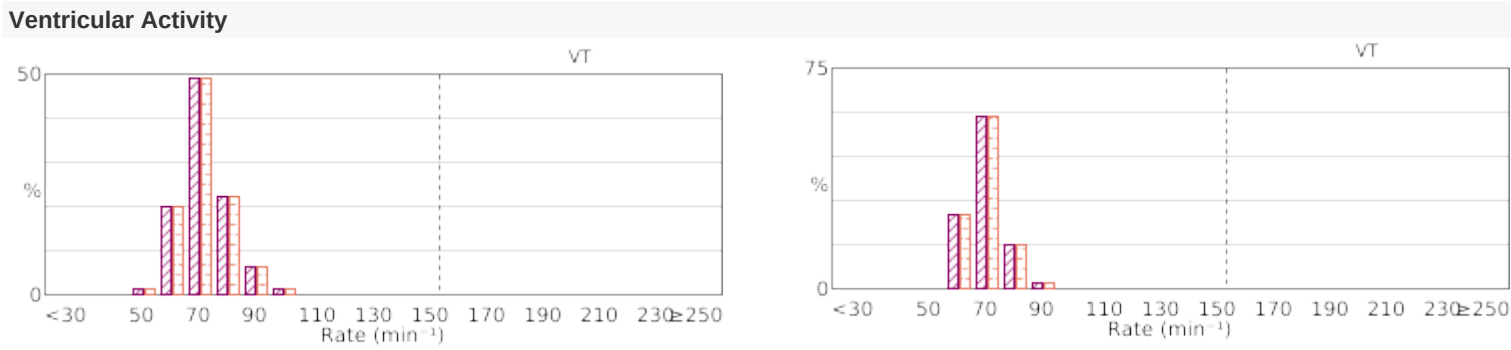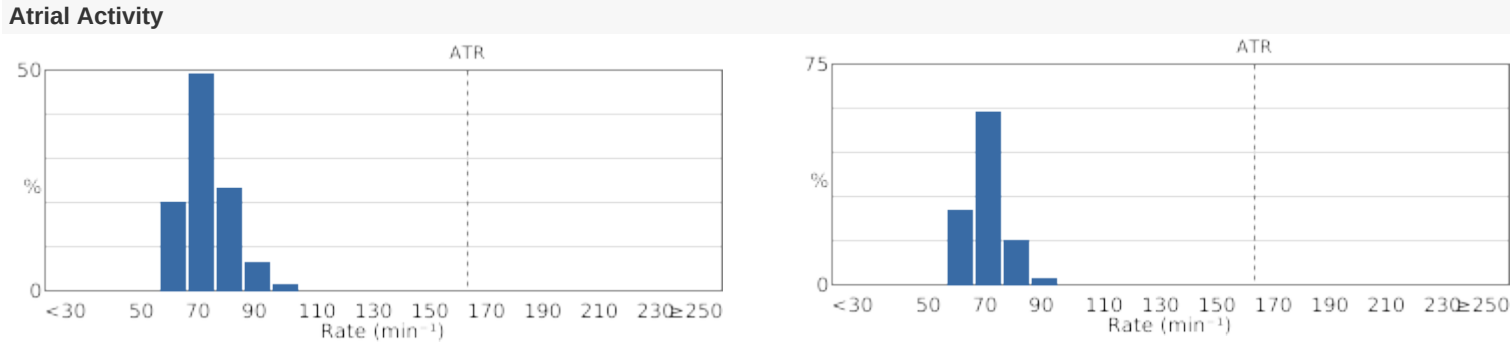

Histogram Rate Counts

Reset Before Last 1042 day(s) 26 Jun 2019 to 03 May 2022			Since Last Reset 25 day(s) 03 May 2022 to 29 May 2022	
Atrial				
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	0	141	0	0
30-39	0	59.8K	0	252
40-49	26	19.1K	0	13
50-59	2.2K	455.7K	3	159
60-69	990	22.7M	22	674.6K
70-79	17.0K	55.8M	567	1.6M
80-89	40.4K	25.5M	959	397.6K
90-99	19.1K	7.1M	484	45.6K
100-109	6.5K	1.2M	75	1.6K
110-119	818	167.1K	0	77
120-129	1	36.9K	0	40
130-139	0	7.2K	0	29
140-149	0	1.5K	0	11
150-159	0	1.3K	0	8
160-169	0	1.7K	0	14
170-179	0	1.8K	0	9
180-189	0	1.6K	0	12
190-199	0	1.3K	0	7
200-209	0	1.2K	0	2
210-219	0	883	0	3
220-229	0	754	0	2
230-239	0	600	0	3
240-249	0	527	0	1
>=250	0	24.4K	0	2

Reset Before Last 1042 day(s) 26 Jun 2019 to 03 May 2022			Since Last Reset 25 day(s) 03 May 2022 to 29 May 2022	
Right Ventricular				
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	0	0	0	0
30-39	0	0	0	0
40-49	11	0	0	0
50-59	660.9K	758	799	2
60-69	22.6M	5.7K	674.2K	322
70-79	55.6M	44.0K	1.6M	870
80-89	25.4M	128.9K	397.8K	649
90-99	7.1M	179.0K	45.9K	472
100-109	1.2M	100.4K	1.7K	158
110-119	162.7K	24.5K	61	63
120-129	14.4K	40.5K	31	86
130-139	0	10.9K	0	37
140-149	0	2.9K	0	19
150-159	0	1.7K	0	23
160-169	0	1.3K	0	9
170-179	0	650	0	8
180-189	0	191	0	3
190-199	0	52	0	0
200-209	0	17	0	0
210-219	0	1	0	0
220-229	0	6	0	0
230-239	0	2	0	0
240-249	0	0	0	0
>=250	0	0	0	0


Reset Before Last 1042 day(s)			Since Last Reset 25 day(s)	
Left Ventricular 26 Jun 2019 to 03 May 2022			03 May 2022 to 29 May 2022	
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	3	440	0	0
30-39	359	11	1	0
40-49	32.3K	509	29	0
50-59	640.4K	898	716	12
60-69	22.6M	13.8K	673.3K	608
70-79	55.5M	47.9K	1.6M	895
80-89	25.4M	118.0K	397.0K	569
90-99	7.1M	143.7K	45.8K	534
100-109	1.2M	125.6K	1.7K	161
110-119	164.5K	49.0K	68	50
120-129	13.3K	36.0K	35	30
130-139	1.2K	7.7K	7	16
140-149	1.6K	1.9K	3	10
150-159	426	1.2K	0	19
160-169	1	811	0	13
170-179	13	436	0	5
180-189	11	208	0	4
190-199	0	82	0	0
200-209	0	24	0	0
210-219	0	4	0	0
220-229	0	2	0	0
230-239	0	1	0	0
240-249	0	0	0	0
>=250	7	0	0	0

Reset Before Last 1042 day(s)			Since Last Reset 25 day(s)	
RV Rate during AT/AF 26 Jun 2019 to 03 May 2022			03 May 2022 to 29 May 2022	
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	0	0	0	0
30-39	0	0	0	0
40-49	0	0	0	0
50-59	0	0	0	0
60-69	0	0	0	0
70-79	1	0	0	0
80-89	8	1	0	0
90-99	829	176	0	0
100-109	2.9K	2.0K	0	0
110-119	862	2.6K	0	0
120-129	16	1.6K	0	0
130-139	0	1.1K	0	0
140-149	0	882	0	0
150-159	0	702	0	0
160-169	0	639	0	0
170-179	0	379	0	0
180-189	0	82	0	0
190-199	0	9	0	0
200-209	0	3	0	0
210-219	0	1	0	0
220-229	0	1	0	0
230-239	0	1	0	0
240-249	0	0	0	0
>=250	0	0	0	0

Heart Rate Variability


Last measured for 24-hr period ending 28 May 2022 17:15

% of Time Used	100
Footprint	19 %
SDANN	54 ms
Mode	DDD
Sensed AV Delay	80 - 120 ms
Ventricular Pacing Chamber	BiV
LV Offset	0 ms

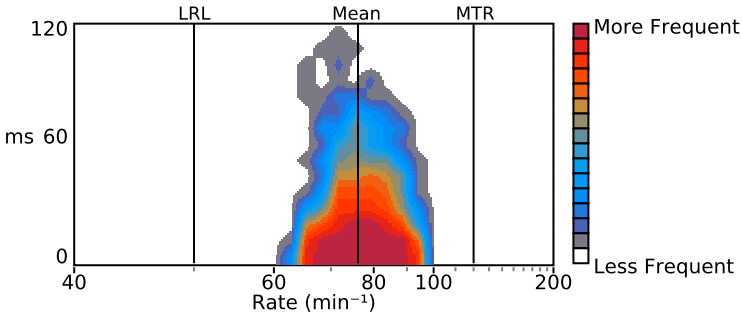


Reference: 24-hr period ending 27 Jun 2019 16:46


% of Time Used	98
Footprint	20 %
SDANN	45 ms
Mode	DDD
Sensed AV Delay	80 - 120 ms
Ventricular Pacing Chamber	BiV
LV Offset	0 ms

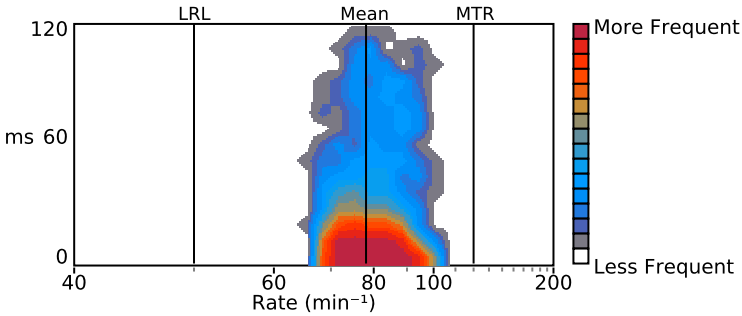


Presenting EGM (29 May 2022)

EGM displayed at 25mm per second

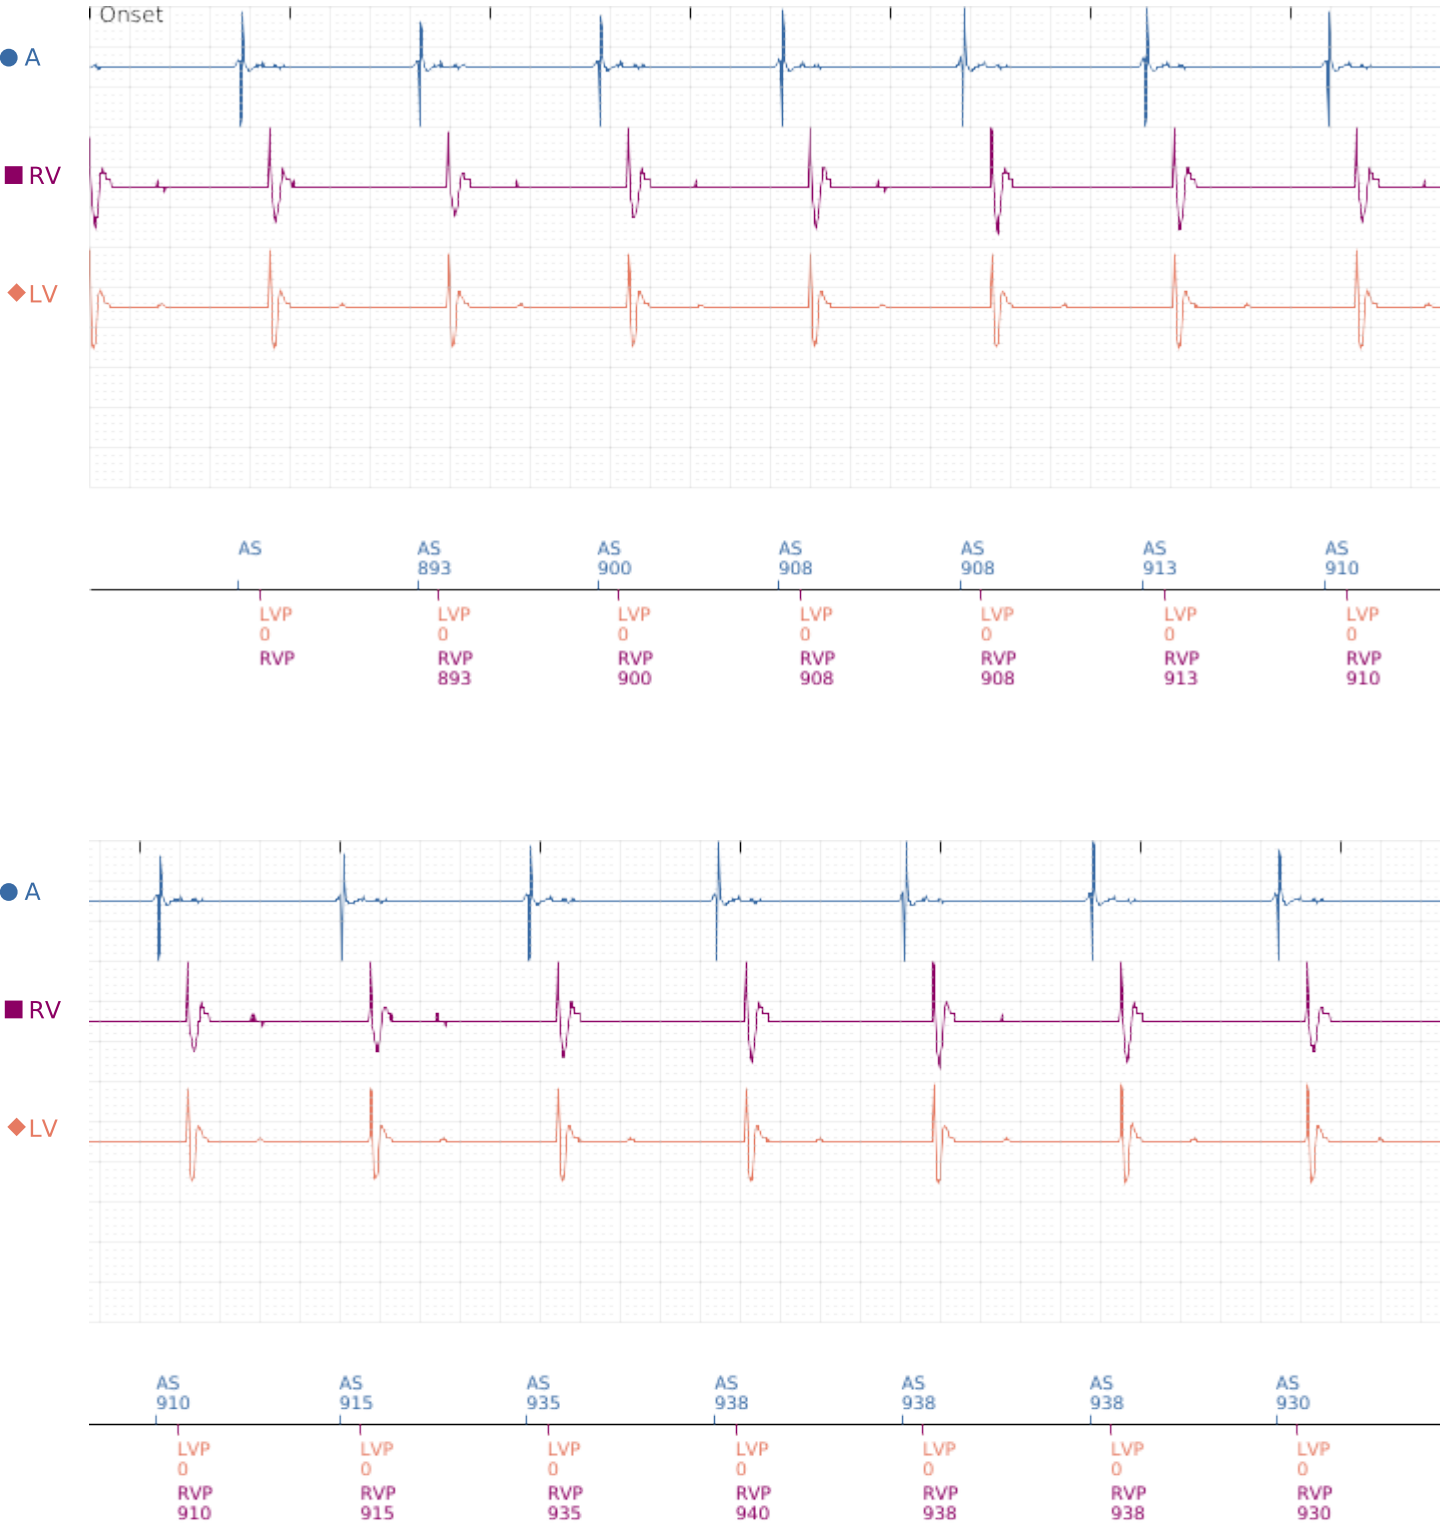

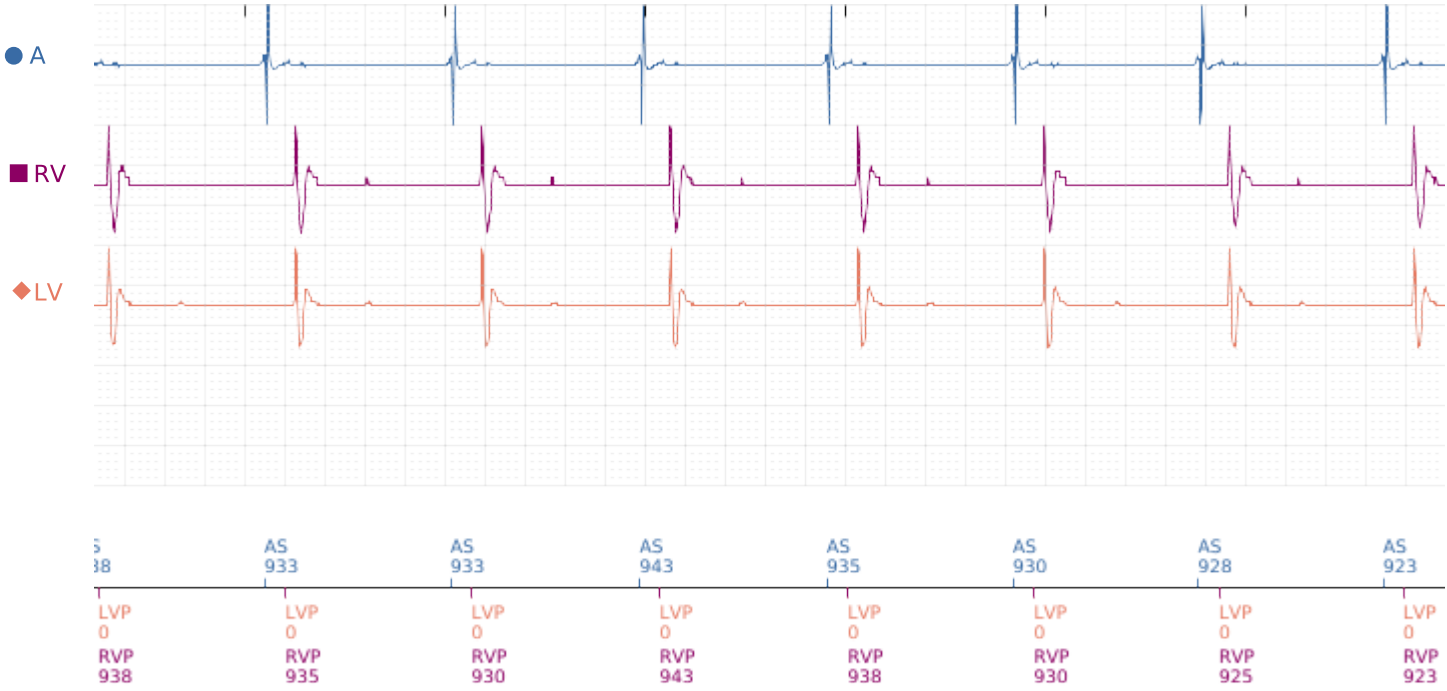

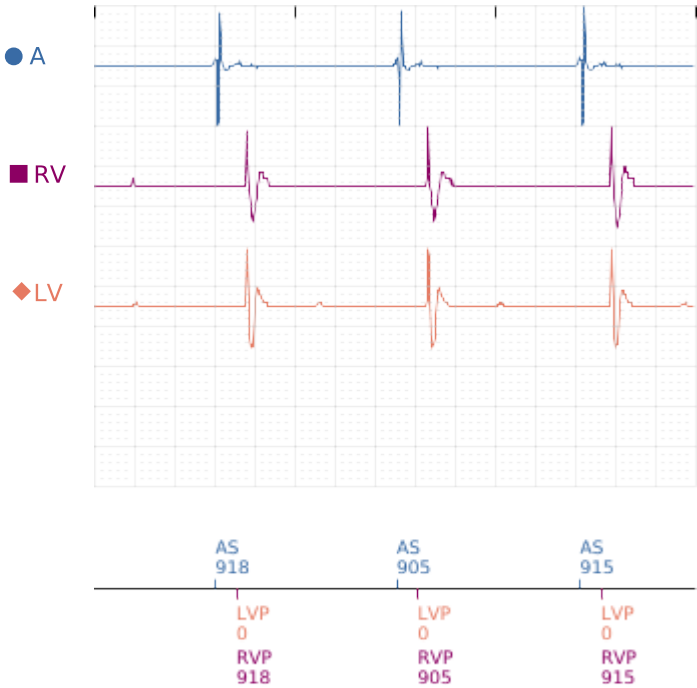

All Events Since Last Reset (03 May 2022)

28 May 2022 13:23 NonSustV at 175 min⁻¹

28 May 2022 08:26 RA Auto

28 May 2022 08:25 RV Auto

03 May 2022 20:26 RA Auto

03 May 2022 20:25 RV Auto

Total Events: 1 NonSustV

Battery (Continued)

Time Since Implant 36 months

Charge Remaining 0.32 ampere-hours

Power Consumption 49 μW

(Measured with programmed parameters)

This device is using 92% of the power it would use at the following parameters:

● A 15% pacing, 70 min⁻¹, 2.5 V, 0.4 ms, 500 Ω

■ RV 100% pacing, 70 min⁻¹, 2.5 V, 0.4 ms, 500 Ω

◆ LV 100% pacing, 70 min⁻¹, 3.5 V, 0.4 ms, 700 Ω