



Date de naissance :
Appareil :
Centre :
Critères de recherche :
Mode Tachy : **Surveill. + Trait.**

Dernière transmission du dispositif : **28 sept. 2015 00:23 CEST**
Dernière interrogation au cabinet : **28 mars 2015**
Date d'implantation : **26 nov. 2014**
Groupe de patients :

V-1: 21 mars 2015 05:17, TV-1, Fréquence A : 142 min⁻¹, Fréquence V : 141 min⁻¹

Détail

TV-1 Début événem.

Fréq. A moy. 142 min⁻¹
Fréq. V moy. 141 min⁻¹
Détection ID de Rythme
Référence 19 mars 2015 23:59
Seuil du RhythmMatch™ 94 %

Lors de la Délect-V

Fréq. A moy. 142 min⁻¹
Fréq. V moy. 142 min⁻¹
Zone de fréquence TV-1
Stabilité 4 ms
Fréquence V>A Faux
Fib A Faux
RhythmID corrélé Vrai
RhythmMatch™ 98 %
DFS satisfaite (Faux, arrêt)
Durée limite ATP Faux

Tentative 1, Pas de traitement V

Temps écoulé 00:00:03

Informations tentative



Traitement tachy désactivé.

Fin de l'événement

00:01:06

EGM affiché à 25 mm par seconde



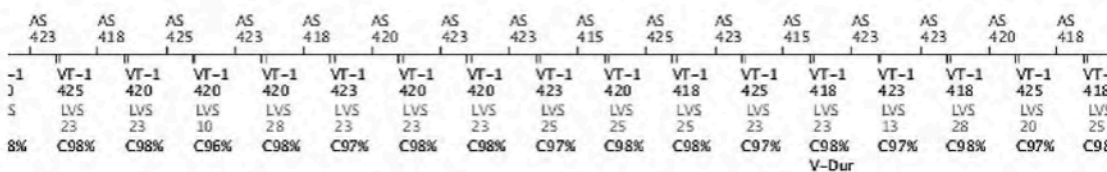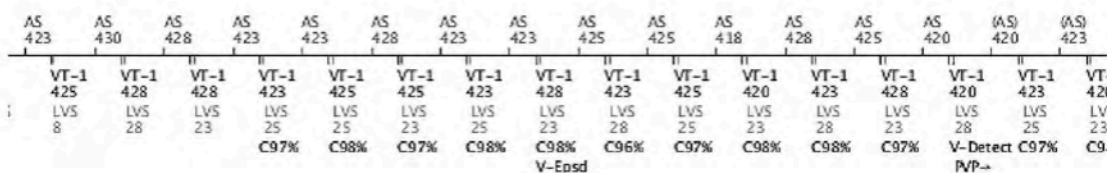


● A



■ VD



Choc



AS	AS	AS	AS	AS	AS	AS	AS	AS	AS	AS	AS	AS	AS	AS	AS	AS
423	428	418	420	423	423	420	423	423	425	420	423	428	420	425	425	
-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-1	VT-
423	420	423	423	420	423	423	423	420	425	423	423	423	425	423	425	42-
LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS
23	25	23	23	25	23	25	28	23	23	23	23	25	25	23	23	23
3%	C98%	C97%	C97%	C98%	C97%	C97%	C97%	C98%	C98%	C97%	C98%	C97%	C98%	C98%	C98%	C98%

● A



■ VD



Choc



AS	AS	AS	AS
420	425	428	423
-1	VT-1	VT-1	VT-1
423	425	423	423
LVS	LVS	LVS	LVS
25	25	25	25
3%	C96%	C98%	C97%

↑ > Plage V	↓ < Plage V	■ Détection V	□ Stimulatio
↑ > Plage A	↓ < Plage A	• Détection A	○ Stimulatio

