

My Alerts

26 Jun 2025 12:44  Atrial pacing lead impedance out of range.

For Technical Support contact 1-800-CARDIAC (Americas) or your local Boston Scientific Representative.

Events Since Last Reset (16 Jun 2025)


26 Jun 2025 12:49 RV Auto

24 Jun 2025 18:49 RV Auto

Battery

Approximate time to explant: 5 months from 27 Jun 2025

Last Capacitor Re-form Charge Time29 May 2025 12:2512.1 sOne Year Remaining

Explant 

See last page for additional battery information.

Leads	Implant (28 Sep 2016)	Most Recent In-Office Measurement (16 Jun 2025)	Most Recent Daily Measurement (26 Jun 2025)
Atrial			
Intrinsic Amplitude	N/R	7.5 mV	N/R
Pace Impedance	N/R	1304 Ω	 2399 Ω
Pace Threshold	N/R @ 0.4 ms	2.5 V @ 0.4 ms	N/R
Right Ventricular			
Intrinsic Amplitude	N/R	20.3 mV	N/R
Pace Impedance	N/R	393 Ω	397 Ω
Pace Threshold	N/R @ 0.4 ms	2.1 V @ 0.4 ms	1.8 V @ 0.4 ms
Left Ventricular			
Intrinsic Amplitude	N/R	12.7 mV	N/R
Pace Impedance	N/R	391 Ω	340 Ω
Pace Threshold	N/R @ 0.4 ms	1.3 V @ 0.4 ms	N/R
Shock			
Shock Impedance	N/R	73 Ω	69 Ω


Settings


Ventricular Tachy			
VF	220 min ⁻¹	ATP	41 J, 41 J, 41 Jx6
VT	180 min ⁻¹	Scan	ATP2 Off41 J, 41 J, 41 Jx4
VT-1	110 min ⁻¹	Monitor Only	
Atrial Tachy		Pacing Output	
ATR Mode Switch	170 min ⁻¹	VDI	Atrial2.5 V @ 0.4 ms
Brady/CRT			Right VentricularTrend 2.5 V @ 0.4 ms
Mode	DDD		Left Ventricular3.0 V @ 0.4 ms
Lower Rate Limit	70 min ⁻¹	Sensitivity	
Maximum Tracking Rate	100 min ⁻¹	Atrial	AGC 0.25 mV
Paced AV Delay	90 - 150 ms	Right Ventricular	AGC 0.6 mV
Sensed AV Delay	70 - 120 ms	Left Ventricular	AGC 1.0 mV
A-Refractory (PVARP)	240 - 280 ms	Leads Configuration (Pace/Sense)	
RV-Refractory (RVRP)	210 - 210 ms	Atrial	Bipolar
LV-Refractory (LVRP)	250 ms	Right Ventricular	Bipolar
Ventricular Pacing Chamber	BiV	Left Ventricular	LVtip>>Can/LVtip>>LVring
LV Offset	-40 ms	Rate Adaptive Pacing	
		Minute Ventilation	 Disabled
		Accelerometer	Passive


Rhythm ID Update

Last Successful Completion

N/R





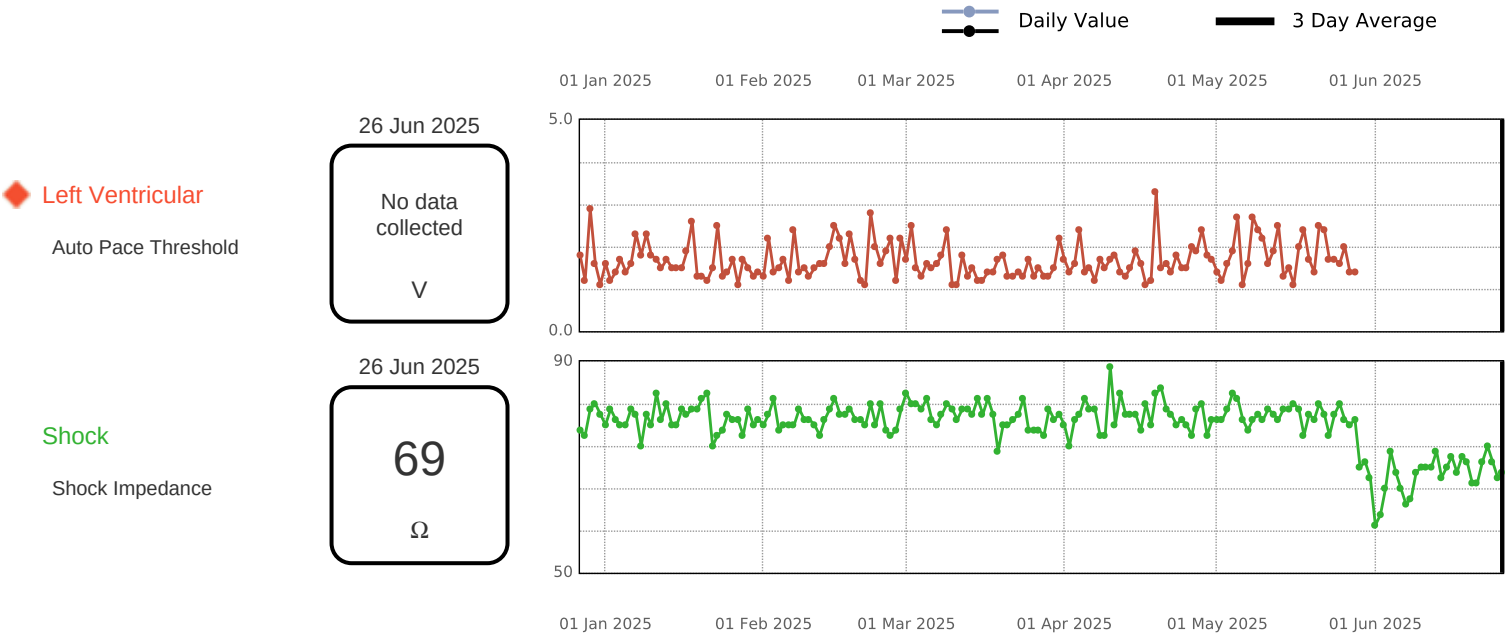

Brady/CRT Counters	Reset Before Last 3183 day(s) 28 Sep 2016 to 16 Jun 2025	Since Last Reset 10 day(s) 16 Jun 2025 to 27 Jun 2025
Counters		
% A Paced	94	98
% RV Paced	99	99
% LV Paced	99	98
Intrinsic Promotion		
Rate Hysteresis		
% Successful	0	0
Atrial Arrhythmia		
% AT/AF (One Year of Data)	<1	0
Total Time in AT/AF (days) (One Year of Data)	2.5	0.0
Episodes by Duration		
< 1 minute	126	0
1 min - < 1 hr	50	0
1 hr - < 24 hr	1	0
24 hr - < 48 hr	3	0
> 48 hr	0	0
Total PACs	216980	7539
Ventricular Counters		
Total PVCs	2467501	2329
Three or More PVCs	1954	1
Clinical Counters	Since Last Reset 16 Jun 2025	Device Totals
MRI Protection Mode	0	0

Histograms



◆ LV


Paced

Sensed


Reset Before Last
3183 day(s)
28 Sep 2016 to 16 Jun 2025

Since Last Reset
10 day(s)
16 Jun 2025 to 27 Jun 2025


Atrial Activity

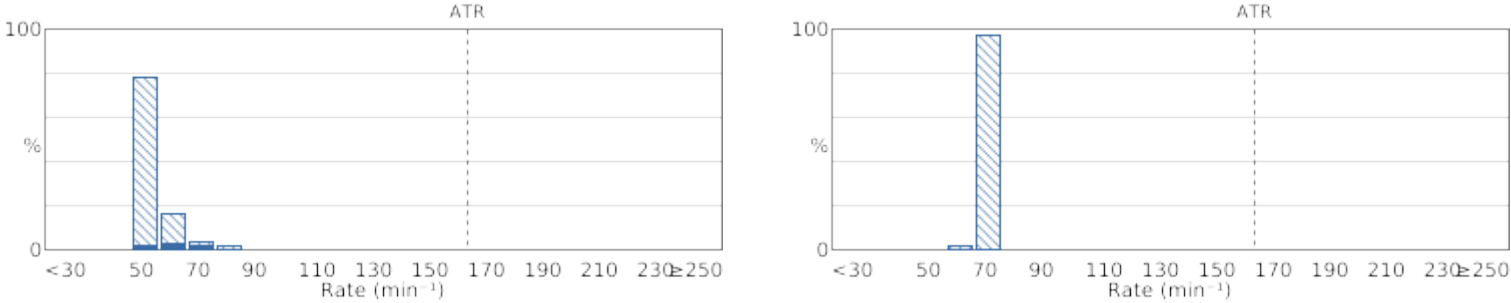


Ventricular Activity

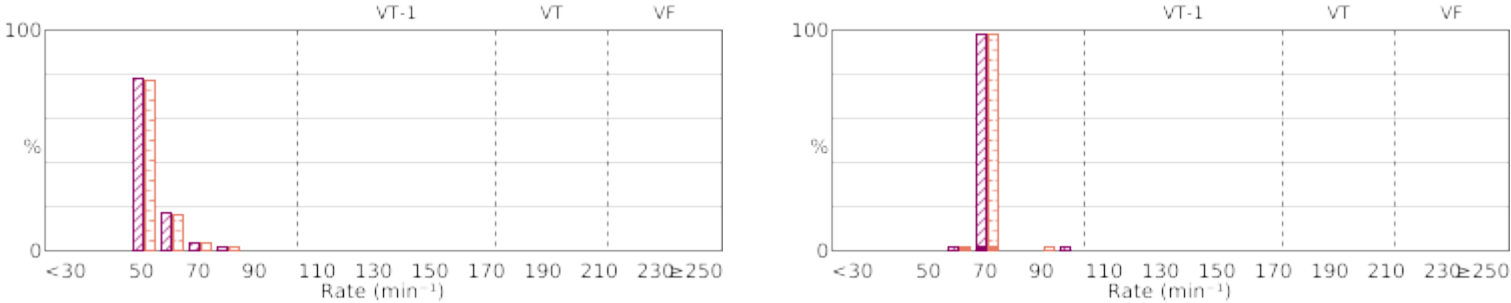

Ventricular Response to Atrial Pace

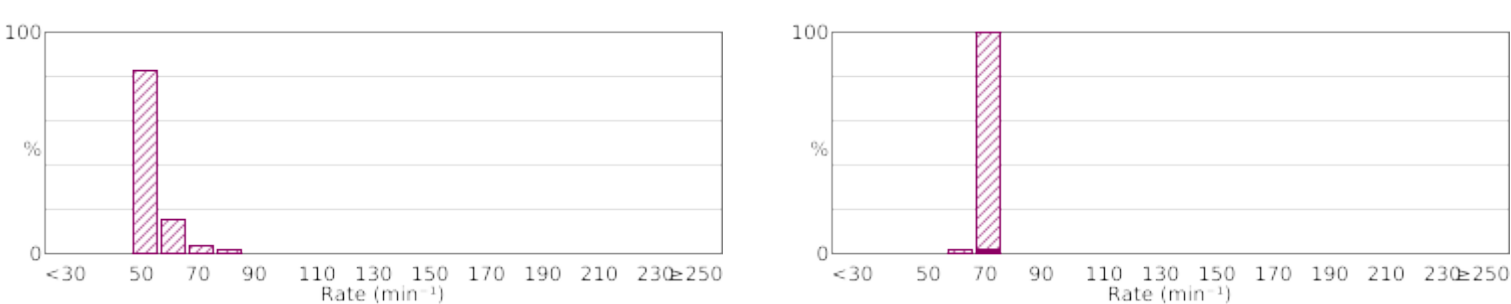

Ventricular Response to Atrial Sense

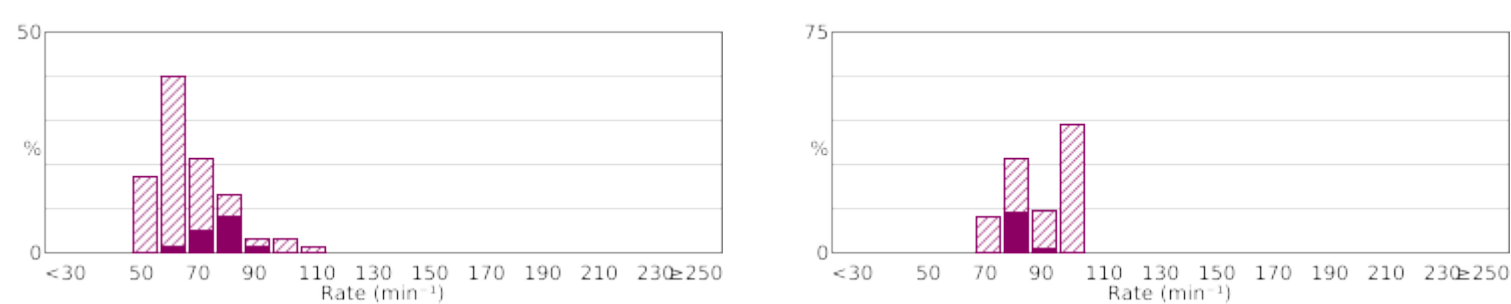

Histogram Rate Counts

Reset Before Last 3183 day(s) 28 Sep 2016 to 16 Jun 2025			Since Last Reset 10 day(s) 16 Jun 2025 to 27 Jun 2025	
Atrial				
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	1	3.0K	0	1
30-39	4	619.7K	0	52
40-49	1.3K	1.0M	0	1.2K
50-59	200.8M	3.1M	2.6K	195
60-69	37.5M	6.0M	10.5K	2
70-79	6.3M	1.9M	1.0M	1.8K
80-89	2.0M	670.8K	0	2.7K
90-99	25.8K	197.7K	0	1.5K
100-109	2.5K	81.2K	0	2.0K
110-119	616	28.8K	0	1.5K
120-129	36.1K	25.6K	0	795
130-139	109.5K	28.1K	0	523
140-149	0	31.0K	0	449
150-159	0	26.0K	0	636
160-169	0	22.8K	0	923
170-179	0	20.7K	0	717
180-189	0	26.2K	0	421
190-199	0	34.3K	0	286
200-209	0	23.9K	0	195
210-219	0	18.9K	0	129
220-229	0	29.0K	0	106
230-239	0	37.6K	0	87
240-249	0	60.4K	0	69
>=250	0	1.2M	0	247

Reset Before Last 3183 day(s) 28 Sep 2016 to 16 Jun 2025			Since Last Reset 10 day(s) 16 Jun 2025 to 27 Jun 2025	
Right Ventricular				
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	0	82	0	0
30-39	44	116	0	0
40-49	1.3K	957	0	0
50-59	204.8M	45.9K	0	0
60-69	43.6M	174.8K	7.5K	0
70-79	8.8M	786.6K	1.0M	7.5K
80-89	2.8M	1.3M	3.0K	2.1K
90-99	354.7K	237.9K	2.1K	181
100-109	504.6K	36.1K	6.9K	6
110-119	241.1K	24.8K	0	9
120-129	54.9K	12.5K	0	4
130-139	153.0K	33.5K	0	0
140-149	55	11.1K	0	1
150-159	88	4.7K	0	0
160-169	39	1.9K	0	0
170-179	15	702	0	0
180-189	5	365	0	0
190-199	3	281	0	0
200-209	3	226	0	0
210-219	3	249	0	0
220-229	4	231	0	0
230-239	4	215	0	0
240-249	2	120	0	0
>=250	61	798	0	0

Left Ventricular	Reset Before Last 3183 day(s)		Since Last Reset 10 day(s)	
	28 Sep 2016 to 16 Jun 2025		16 Jun 2025 to 27 Jun 2025	
Rate (min ⁻¹)	Paced	Sensed	Paced	Sensed
0-29	267	2.9K	0	40
30-39	1.8K	214	0	0
40-49	37.9K	861	0	0
50-59	204.4M	66.9K	35	0
60-69	43.4M	274.2K	3.8K	7.5K
70-79	8.7M	1.2M	1.0M	7.5K
80-89	2.8M	867.1K	4.1K	68
90-99	411.4K	222.2K	8.3K	89
100-109	428.9K	62.2K	129	14
110-119	211.3K	29.4K	275	1
120-129	113.0K	14.2K	463	4
130-139	165.9K	36.6K	0	0
140-149	1.7K	17.0K	0	0
150-159	158	7.2K	0	0
160-169	37	2.1K	0	0
170-179	15	884	0	0
180-189	6	705	0	0
190-199	6	2.2K	0	0
200-209	3	2.3K	0	0
210-219	3	314	0	0
220-229	2	124	0	0
230-239	2	49	0	0
240-249	2	0	0	0
>=250	54	0	0	0

Heart Rate Variability

Last Measured:


Data unavailable



Reference:


Data unavailable

Presenting EGM (27 Jun 2025)

EGM displayed at 25mm per second

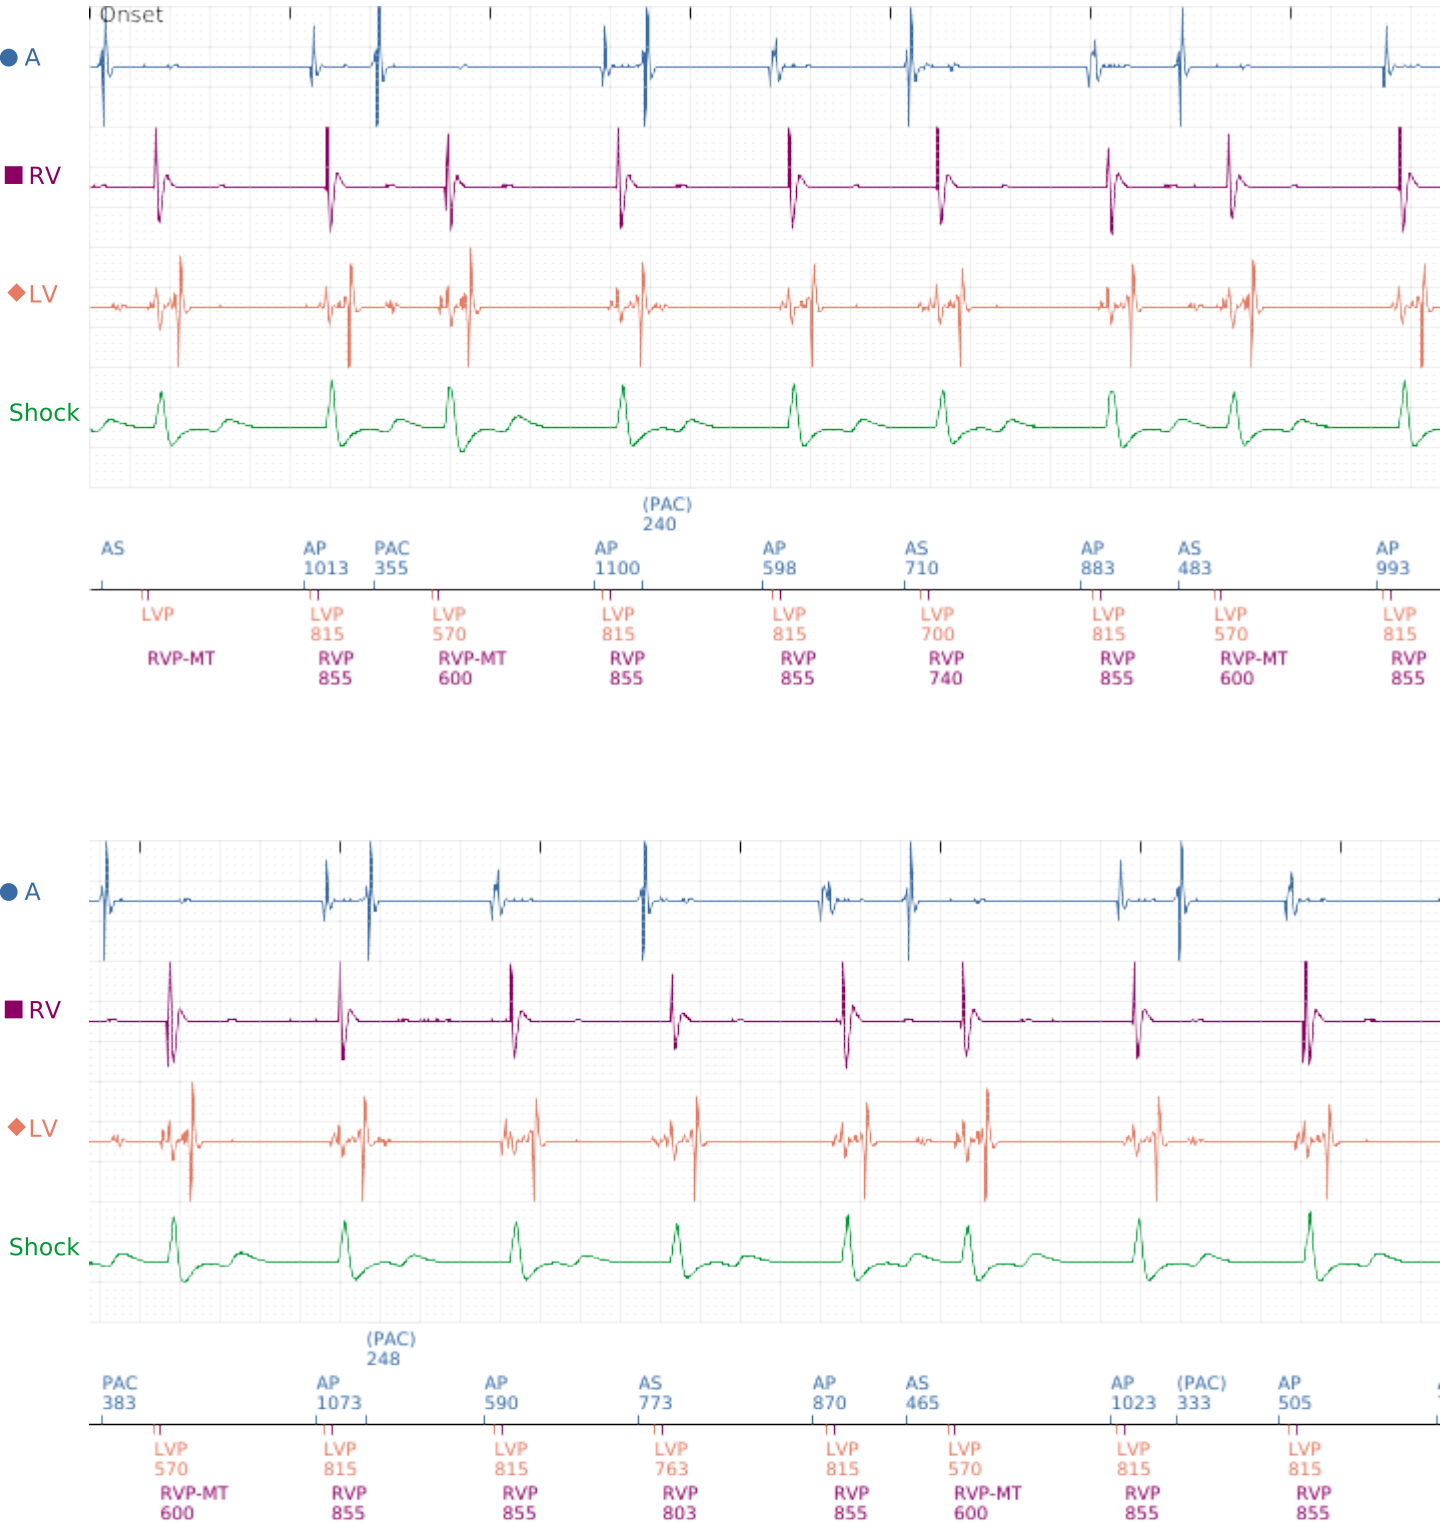

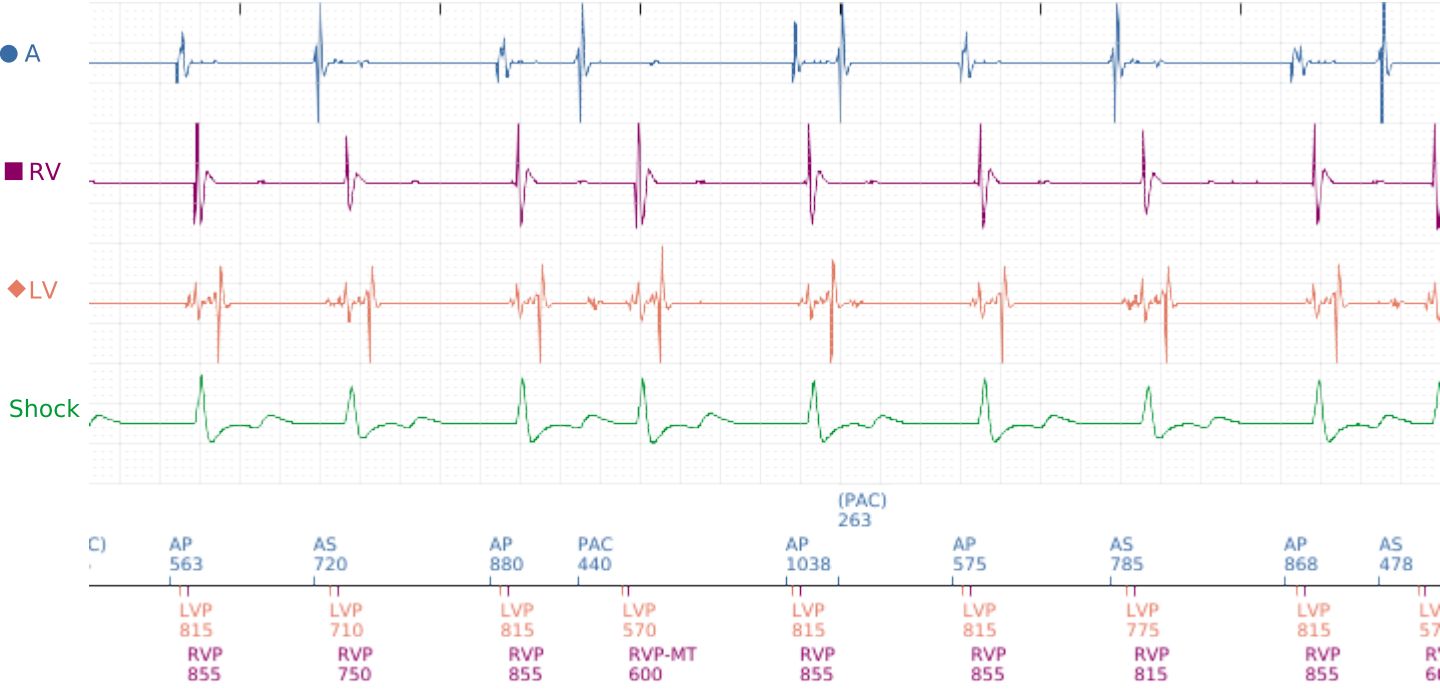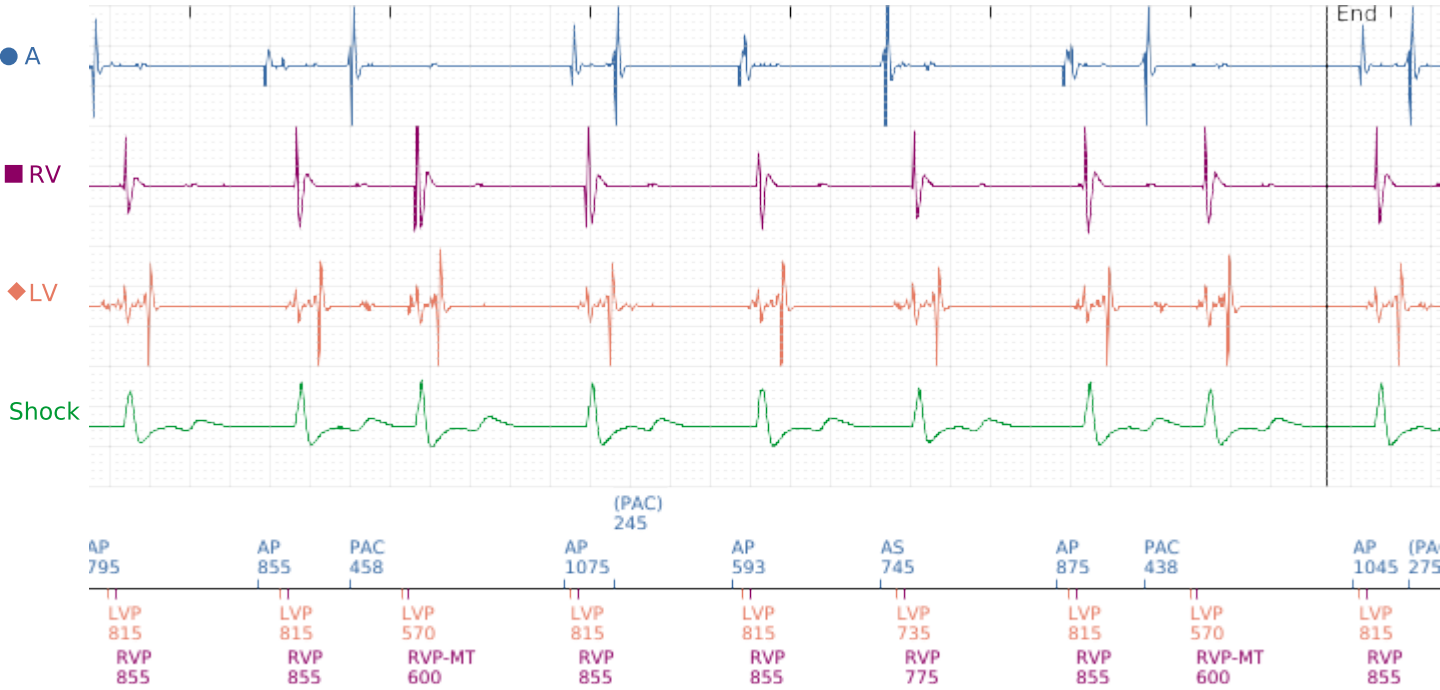

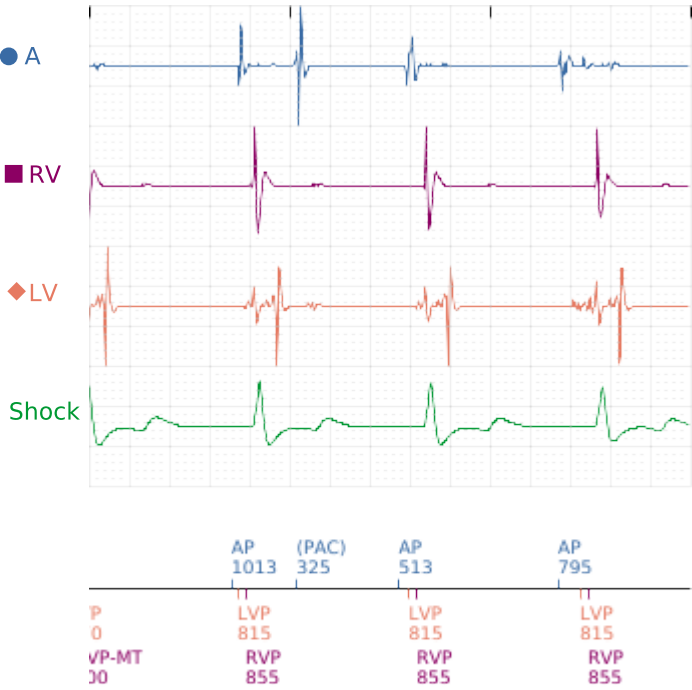

Battery (Continued)			
Last Delivered Shock	29 May 2025 12:31	Time Since Implant	106 months
Energy	41 J	Charge Remaining	0.35 ampere-hours
Charge Time	8.9 s	Power Consumption	72 μW
Shock Impedance	67 Ω	(Measured with programmed parameters)	
Beep when Explant is Indicated	On	This device is using 134% of the power it would use at the following parameters:	
		● A	15% pacing, 70 min ⁻¹ , 2.5 V, 0.4 ms, 500 Ω
		■ RV	100% pacing, 70 min ⁻¹ , 2.5 V, 0.4 ms, 700 Ω
		◆ LV	100% pacing, 70 min ⁻¹ , 3.5 V, 0.4 ms, 700 Ω