



1527

Date of Birth:
Device: **RESONATE CRT-D G424/518110**
Clinic: **CHU Haut Leveque Bordeaux HOPIT**
Search Tags:
Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **21 Aug 2025 13:05 CEST**
Last Office Interrogation: **24 Jul 2025**
Implant Date: **01 Dec 2024**
Patient Group: **TACHY_CHU de Bordeaux (Primary)**

My Alerts

There are no alerts to display.

Events Since Last Reset (01 Apr 2025)

21 Aug 2025 04:09 LV Auto
21 Aug 2025 04:08 RV Auto
See last page for full list of Events Since Last Reset.

Battery OK

Approximate time to explant: **8 years** from 21 Aug 2025

Last Capacitor Re-form

29 Mar 2025 09:55

Charge Time

10.0 s

One Year Remaining

Explant



See last page for additional battery information.

Leads	Implant (01 Dec 2024)	Most Recent In-Office Measurement (18 Jul 2025)	Most Recent Daily Measurement (21 Aug 2025)
Atrial			
Intrinsic Amplitude	6.0 mV	8.0 mV	N/R
Pace Impedance	800 Ω	551 Ω	515 Ω
Pace Threshold	0.4 V @ 0.4 ms	0.8 V @ 0.4 ms	0.6 V @ 0.4 ms
Right Ventricular			
Intrinsic Amplitude	N/R	10.5 mV	N/R
Pace Impedance	700 Ω	595 Ω	633 Ω
Pace Threshold	0.5 V @ 0.4 ms	0.5 V @ 0.4 ms	0.5 V @ 0.4 ms
Left Ventricular			
Intrinsic Amplitude	N/R	13.2 mV	N/R
Pace Impedance	850 Ω	413 Ω	320 Ω
Pace Threshold	1.0 V @ 0.4 ms	Auto 0.9 V @ 0.4 ms	4.0 V @ 0.4 ms
Shock			
Shock Impedance	65 Ω	67 Ω	68 Ω


◆ Left Ventricular

Intrinsic Amplitude

21 Aug 2025

Paced

mV

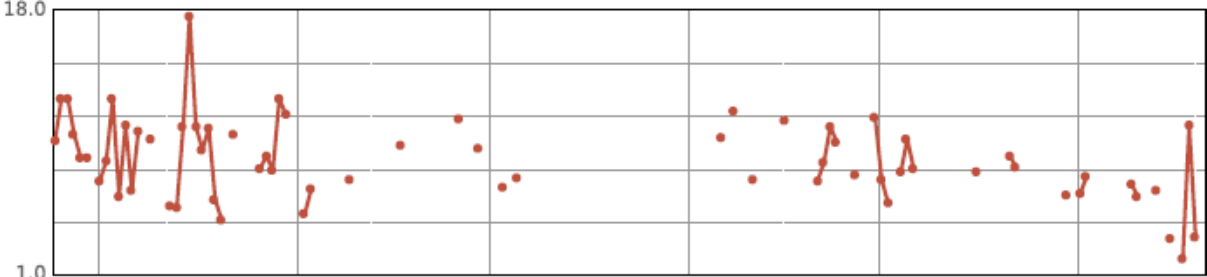


◆ Left Ventricular

Pace Impedance

21 Aug 2025

320

Ω

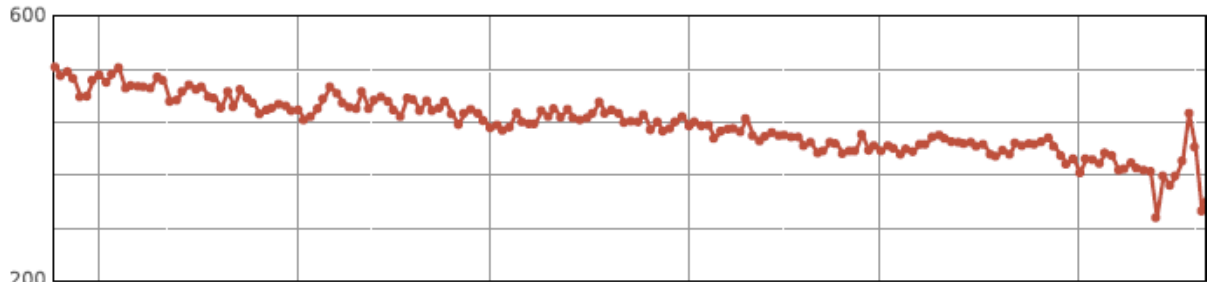


◆ Left Ventricular

Auto Pace Threshold

21 Aug 2025


4.0

V

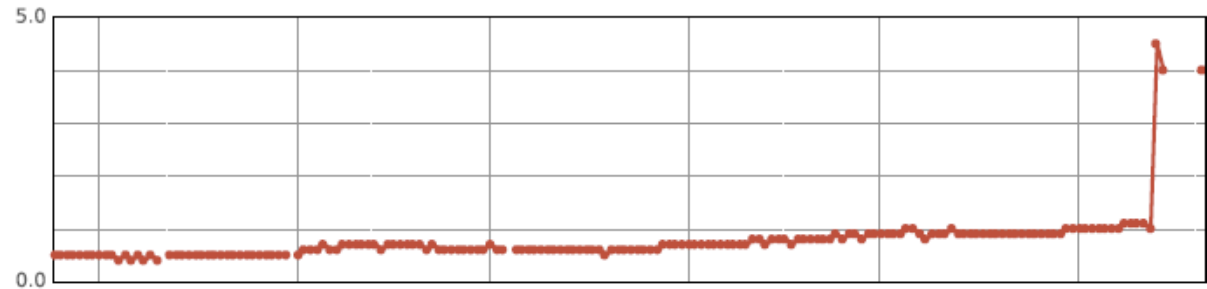


EKG displayed at 25mm per second



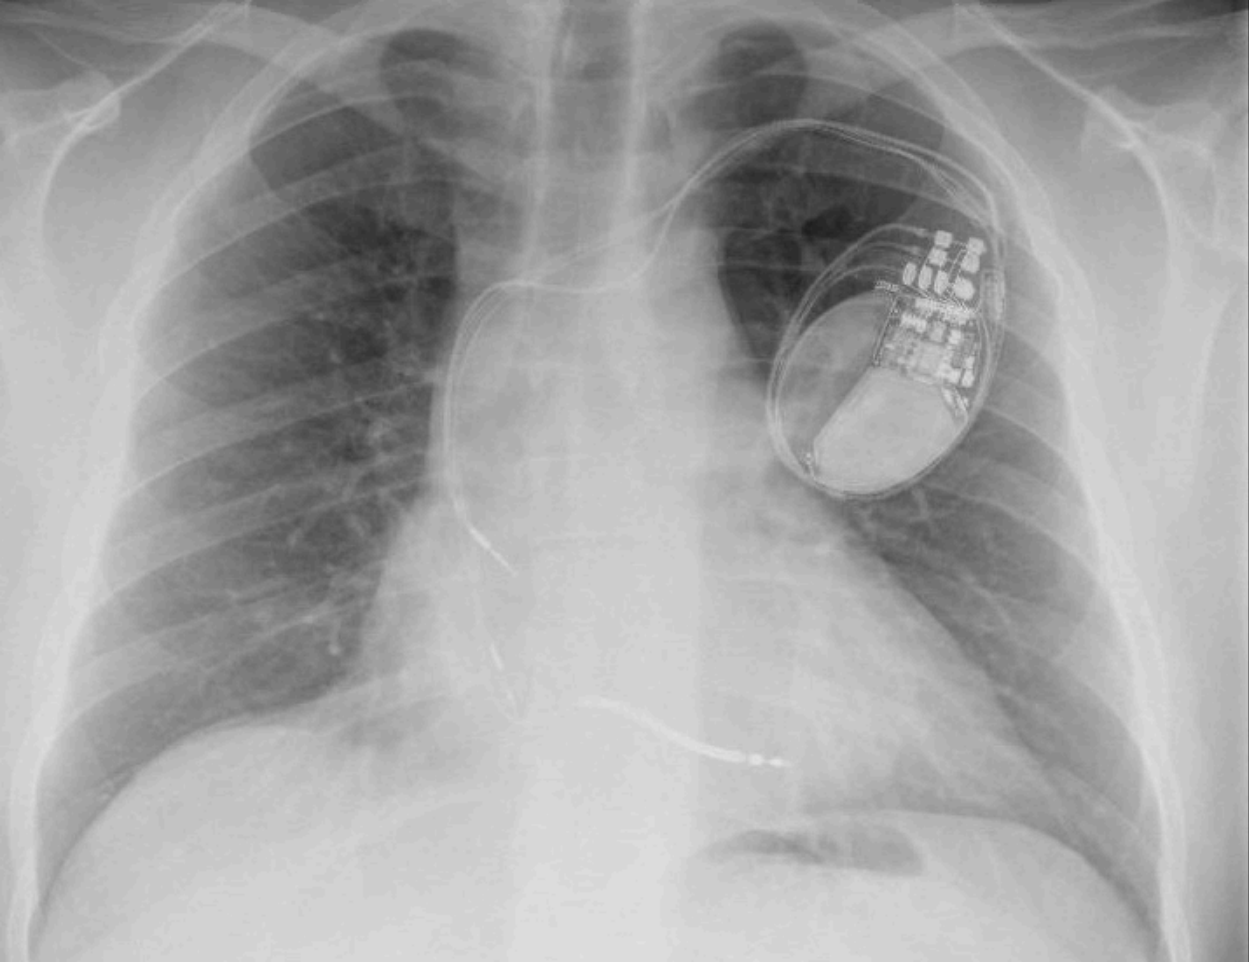

OAG 5°
CAUD 2°

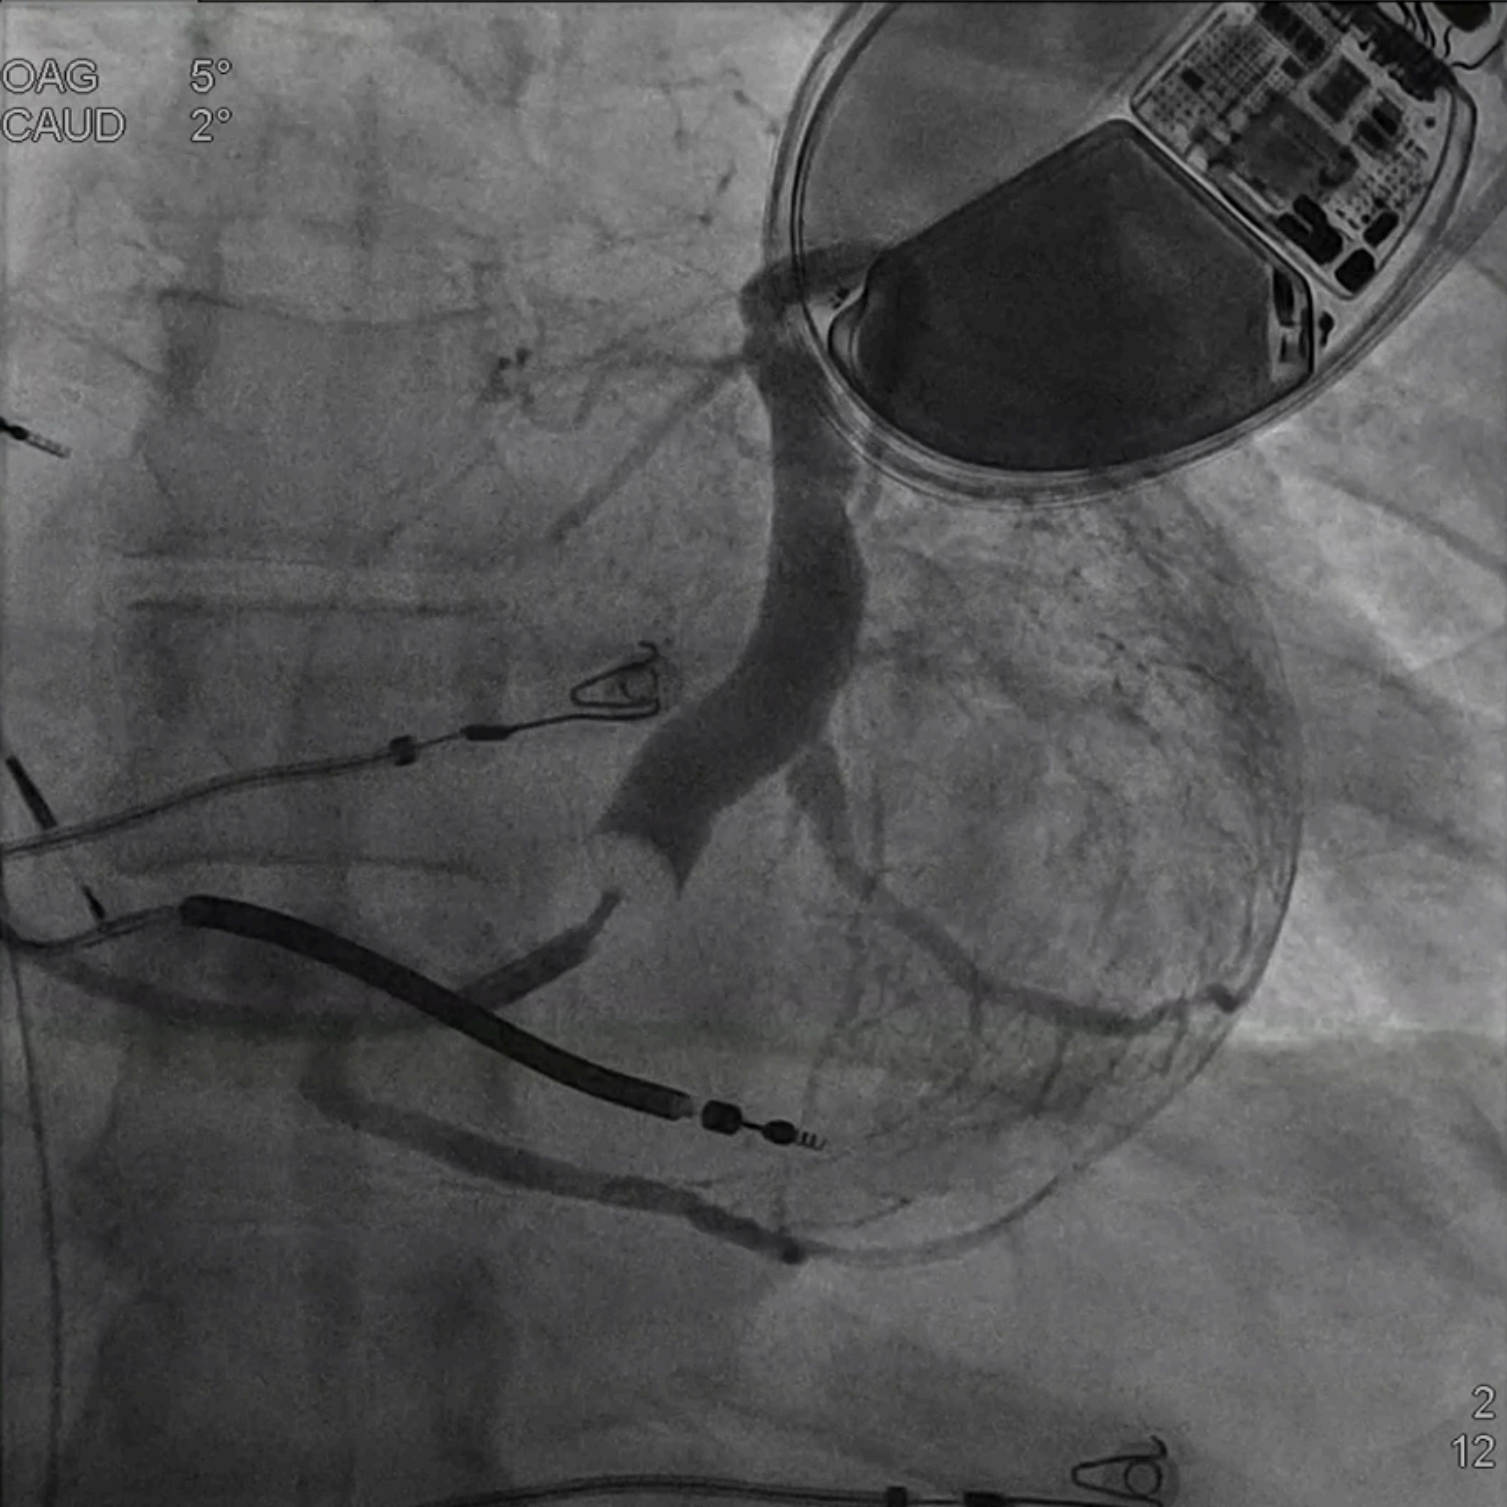

OAG
CAUD

1°
3°

