

My Alerts

12 Sep 2022 14:19



Nonsustained ventricular arrhythmia episode(s).

For Technical Support contact 1-800-CARDIAC (Americas) or your local Boston Scientific Representative.

Events Since Last Reset (25 Nov 2021)

12 Sep 2022 14:21

NonSustV at 152 min⁻¹, Nonsustained

12 Sep 2022 14:20

NonSustV at 146 min⁻¹, Nonsustained

See last page for full list of Events Since Last Reset.

Battery


Approximate time to explant: 9 years from 13 Sep 2022

Last Capacitor Re-form Charge Time

06 Jul 2022 19:29

10.2 s

One Year Remaining

Explant 

Leads	Implant (18 Jan 2019)	Most Recent In-Office Measurement (08 Sep 2022)	Most Recent Daily Measurement (13 Sep 2022)
 Atrial			
Intrinsic Amplitude	N/R	N/R (12 May 2022)	N/R
Pace Impedance	N/R	624 Ω	589 Ω
Pace Threshold	N/R	1.7 V @ 0.4 ms (29 Sep 2021)	N/R
 Right Ventricular			
Intrinsic Amplitude	N/R	3.4 mV	3.7 mV
Pace Impedance	N/R	731 Ω	779 Ω
Pace Threshold	N/R	1.4 V @ 0.4 ms	N/R
 Left Ventricular			
Intrinsic Amplitude	N/R	4.9 mV	5.2 mV
Pace Impedance (LVa)	N/R	393 Ω	367 Ω
Pace Impedance (LVb)		692 Ω	
Pace Threshold	N/R	2.7 V @ 1.0 ms	N/R
 Shock			
Shock Impedance	N/R	59 Ω	51 Ω

Brady/CRT Counters	Since Last Reset 25 Nov 2021
Atrial	0 % Paced
Right Ventricular	8 % Paced
Left Ventricular (LVa)	8 % Paced
Left Ventricular (LVb)	0 % Paced

Atrial Arrhythmia Counters	Since Last Reset 25 Nov 2021
% AT/AF (One Year of Data)	N/R

Ventricular Tachy				
VF	230 min ⁻¹	ATP		41 J, 41 J, 41 Jx6
VT	160 min ⁻¹	Scan	Ramp	41 J, 41 J, 41 Jx4
VT-1	140 min ⁻¹	Monitor Only		
Brady/CRT		Pacing Output		
Mode	VVI	■ Right Ventricular		3.0 V @ 0.4 ms
Lower Rate Limit	40 min ⁻¹	◆ Left Ventricular (LVa)		4.0 V @ 1.0 ms
RV-Refractory (RVRP)	-- - 250 ms	◆ Left Ventricular (LVb)		Off
LV-Refractory (LVRP)	250 ms	Sensitivity		
Ventricular Pacing Chamber	BiV	● Atrial		AGC 0.15 mV
LV Offset	0 ms	■ Right Ventricular		AGC 0.6 mV
		◆ Left Ventricular		AGC 1.0 mV
		Leads Configuration (Pace/Sense)		
		● Atrial		Bipolar
		■ Right Ventricular		Bipolar
		◆ LVa (Pace)		LVRing4>>RV
		◆ LVb (Pace)		Off
		◆ LV (Sense)		LVRing2>>LVRing3
		Rate Adaptive Pacing		
		Minute Ventilation		Passive
		Accelerometer		Passive
		LV MultiSite Pacing		
		Pacing Order		Off

All Events Since Last Reset (25 Nov 2021)	
12 Sep 2022 14:21	NonSustV at 152 min ⁻¹ , Nonsustained
12 Sep 2022 14:20	NonSustV at 146 min ⁻¹ , Nonsustained
12 Sep 2022 14:20	NonSustV at 167 min ⁻¹ , Nonsustained
12 Sep 2022 14:20	NonSustV at 145 min ⁻¹ , Nonsustained
12 Sep 2022 14:19	NonSustV at 155 min ⁻¹ , Nonsustained
13 Dec 2021 12:43	NonSustV at 137 min ⁻¹ , Nonsustained
13 Dec 2021 12:43	NonSustV at 150 min ⁻¹ , Nonsustained
13 Dec 2021 12:42	NonSustV at 152 min ⁻¹ , Nonsustained
Total Events: 8 NonSustV	




Date of Birth:
Device: **MOMENTUM X4 CRT-D**
G138/381540
Clinic: **CHU Haut Leveque Bordeaux HOPIT**
Search Tags:
Tachy Mode: **Monitor + Therapy**


Latest Device Transmission: **13 Sep 2022 14:03 CEST**
Last Office Interrogation: **08 Sep 2022**
Implant Date: **18 Jan 2019**
Patient Group: **PATIENTS INACTIFS (Primary)**

Presenting EGM (13 Sep 2022)


EGM displayed at 25mm per second

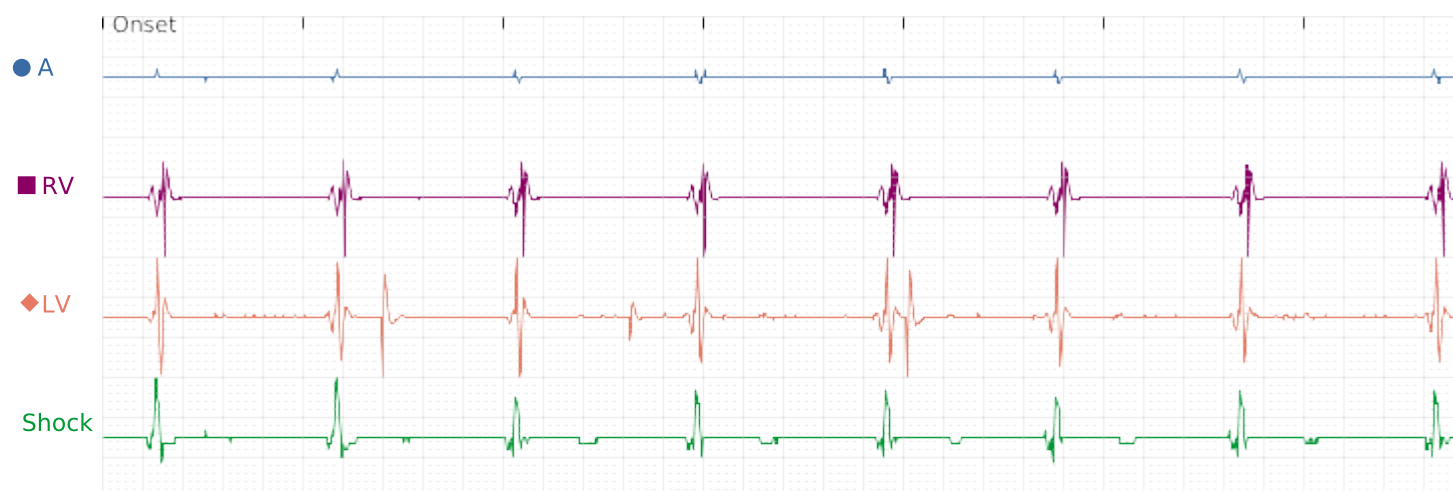

LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS
873	225	890	570	880	918	823	895	94	94
RVS	RVS	RVS	RVS	RVS	RVS	RVS	RVS	RVS	RVS
900	893	905	945	850	923	97			

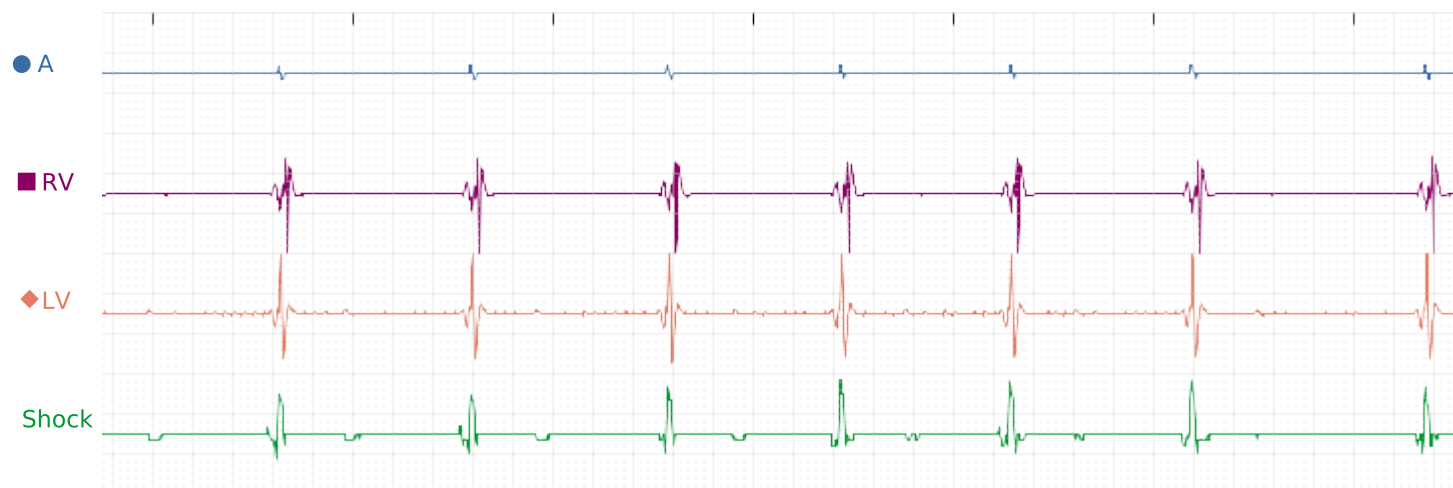

LVS	LVS	LVS	LVS	LVS	LVS	LVS	LVS
948	933	955	835	820	880	114	114
RVS	RVS	RVS	RVS	RVS	RVS	RVS	RVS
975	960	983	863	848	908	116	116

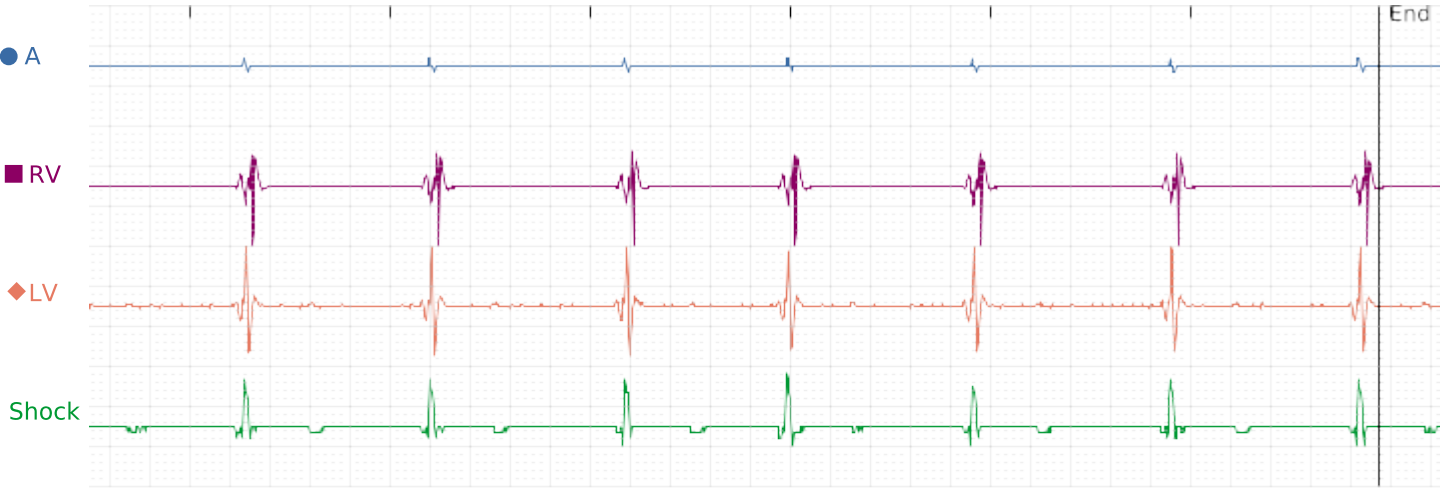

0	LVS 888	LVS 900	LVS 948	LVS 780	LVS 900	LVS 958	LVS 915
5	RVS 915	RVS 928	RVS 975	RVS 808	RVS 930	RVS 985	RVS 943
38							



LVS 955	LVS 920	LVS 945	LVS 860	LVS 875	LVS 900	LVS 955
RVS 983	RVS 950	RVS 975	RVS 890	RVS 905	RVS 928	RVS 985

