



LATITUDE™ Patient Management - Event Detail Report		Report Created: 16 Jan 2023
	Date of Birth:	Latest Device Transmission: 16 Jan 2023 00:50 CET
	Device: MOMENTUM CRT-D	Last Office Interrogation: 07 Oct 2022
	Clinic:	Implant Date:
	Search Tags:	Patient Group:
	Tachy Mode: Monitor + Therapy	



V-5: 01 Mar 2019 21:09, VF, A Rate: 90 min⁻¹, V Rate: 210 min⁻¹

Detail

VF Event Onset			
Avg A Rate	90 min ⁻¹		
Avg V Rate	210 min ⁻¹		
Detection	Rhythm ID		
Template	26 Feb 2019 06:43		
RhythmMatch™ Threshold	94 %		
At V-Detect			
Avg A Rate	89 min ⁻¹	Attempt 1, Burst V ATP	
Avg V Rate	205 min ⁻¹	Elapsed Time	00:00:03
Rate Zone	VT	ATP Information	
Stability	7 ms	Number of Bursts	1
V>A Rate	True		
AFib	False		
RhythmID Correlated	False		
RhythmMatch™	0 %		
SRD Met	False		
ATP Timeout	False		
Attempt 2, 41 J V Shock			
At V-Detect		Elapsed Time	00:00:10
Avg A Rate	85 min ⁻¹	Shock Information	
Avg V Rate	201 min ⁻¹	Charge Time	9.4 s
Rate Zone	VF	Lead Impedance	77 Ω
ATP Timeout	False	Lead Polarity	Initial
Event Ended			00:00:51
EGM displayed at 25mm per second			

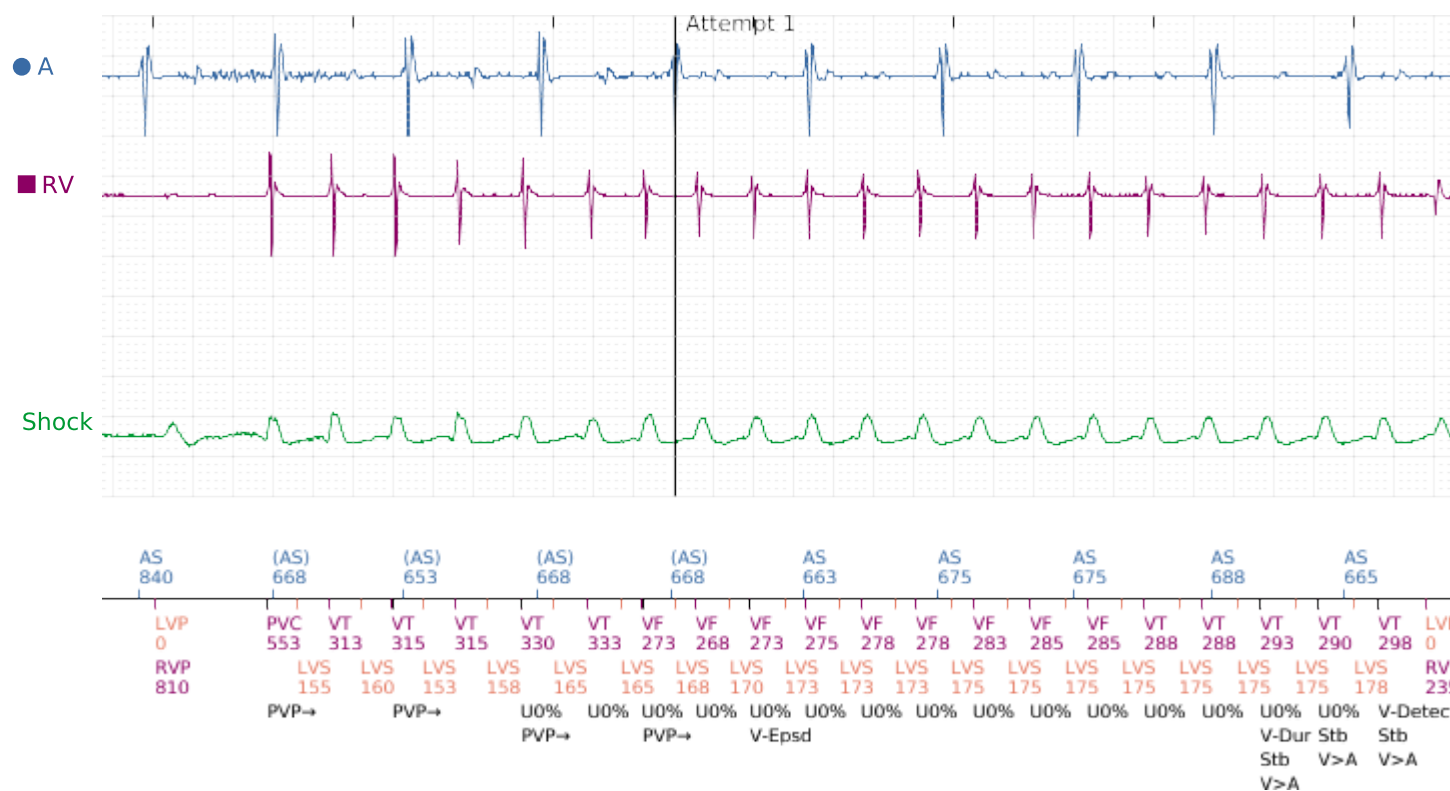

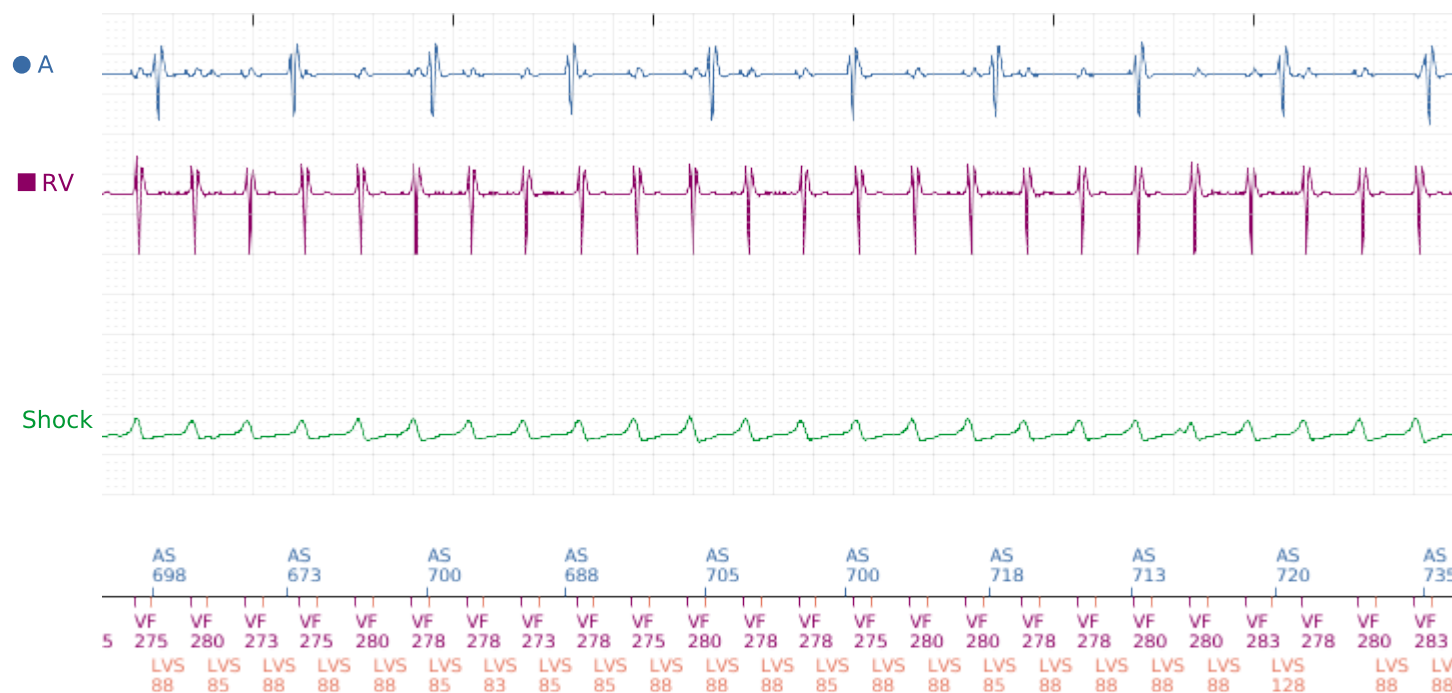

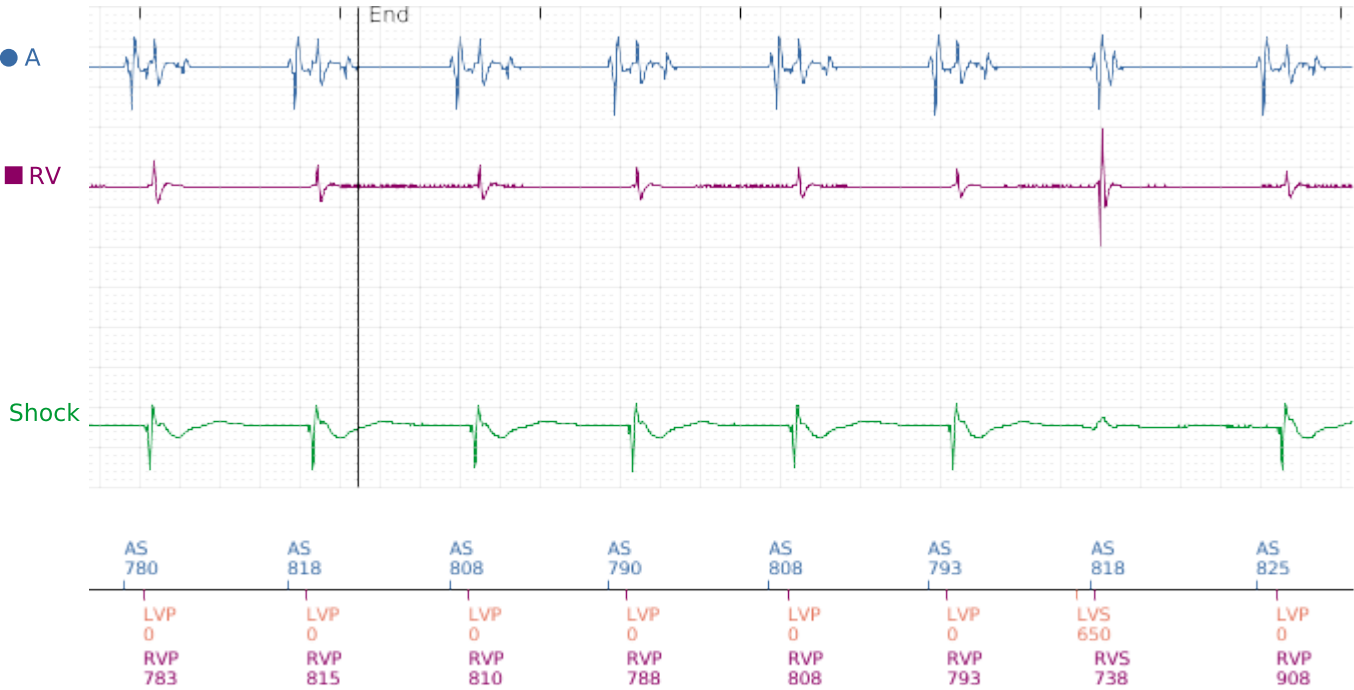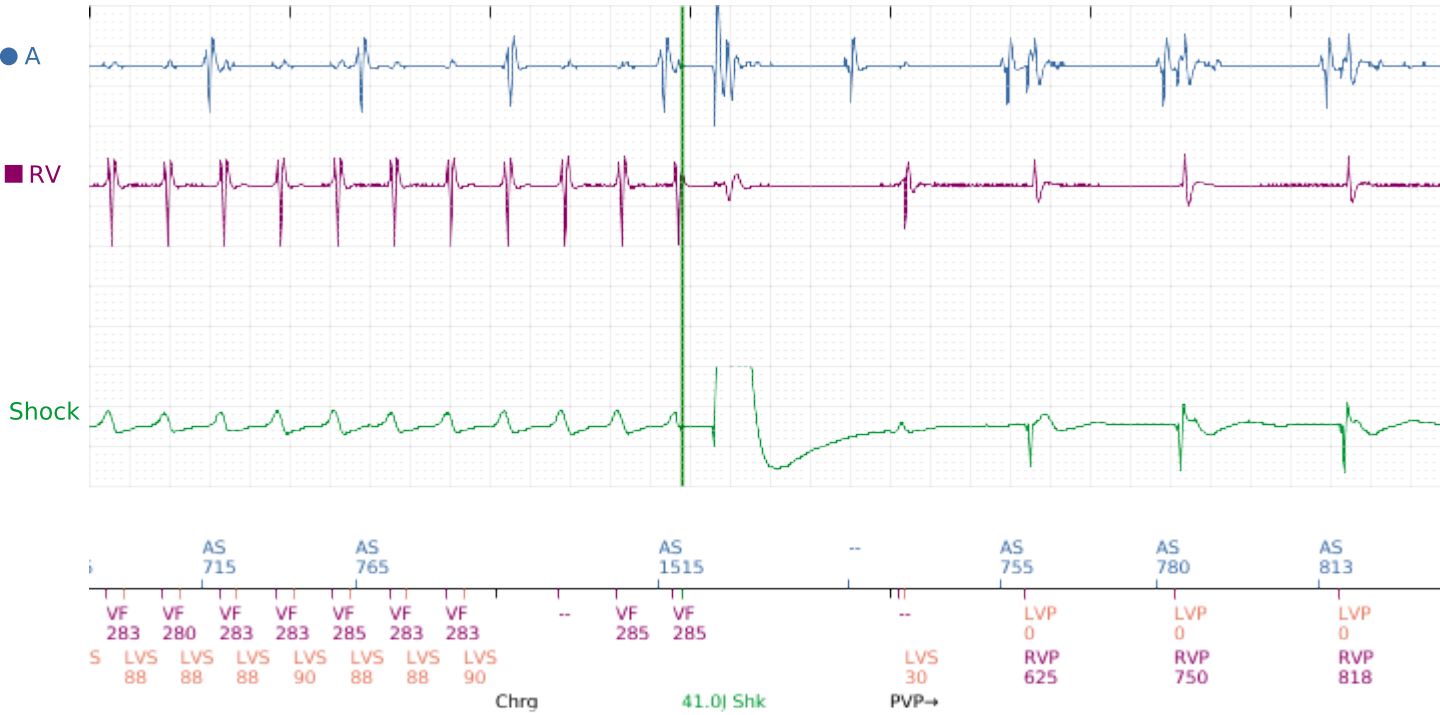

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

