



Date of Birth: _____
Device: **RESONATE X4 CRT-D**

Latest Device Transmission: **02 May 2022 02:31 CEST**
Last Office Interrogation: **05 Oct 2020**
Implant Date:

Clinic:
Search Tags:
Tachy Mode: **Monitor + Therapy**

V-1: 14 Oct 2020 18:18, VF, A Rate: 300 min⁻¹, V Rate: 254 min⁻¹

Detail

VF Event Onset

Avg A Rate	300 min ⁻¹
Avg V Rate	254 min ⁻¹
Detection	Rate Only
Template	10 Aug 2020 07:25

At V-Detect

Avg A Rate	237 min ⁻¹
Avg V Rate	276 min ⁻¹
Rate Zone	VF
Stability	(15 ms, Off)
V>A Rate	(True, Off)
AFib	(True, Off)
RhythmMatch™	Too Fast
SRD Met	(False, Off)
ATP Timeout	False
Onset Intvl	(235 ms, Off)
Onset %	(41 %, Off)


Attempt 1, 41 J V Shock


Elapsed Time	00:00:05
Shock Information	
Charge Time	11.0 s
Lead Impedance	64 Ω
Lead Polarity	Initial

Event Ended


00:00:48

EGM displayed at 25mm per second

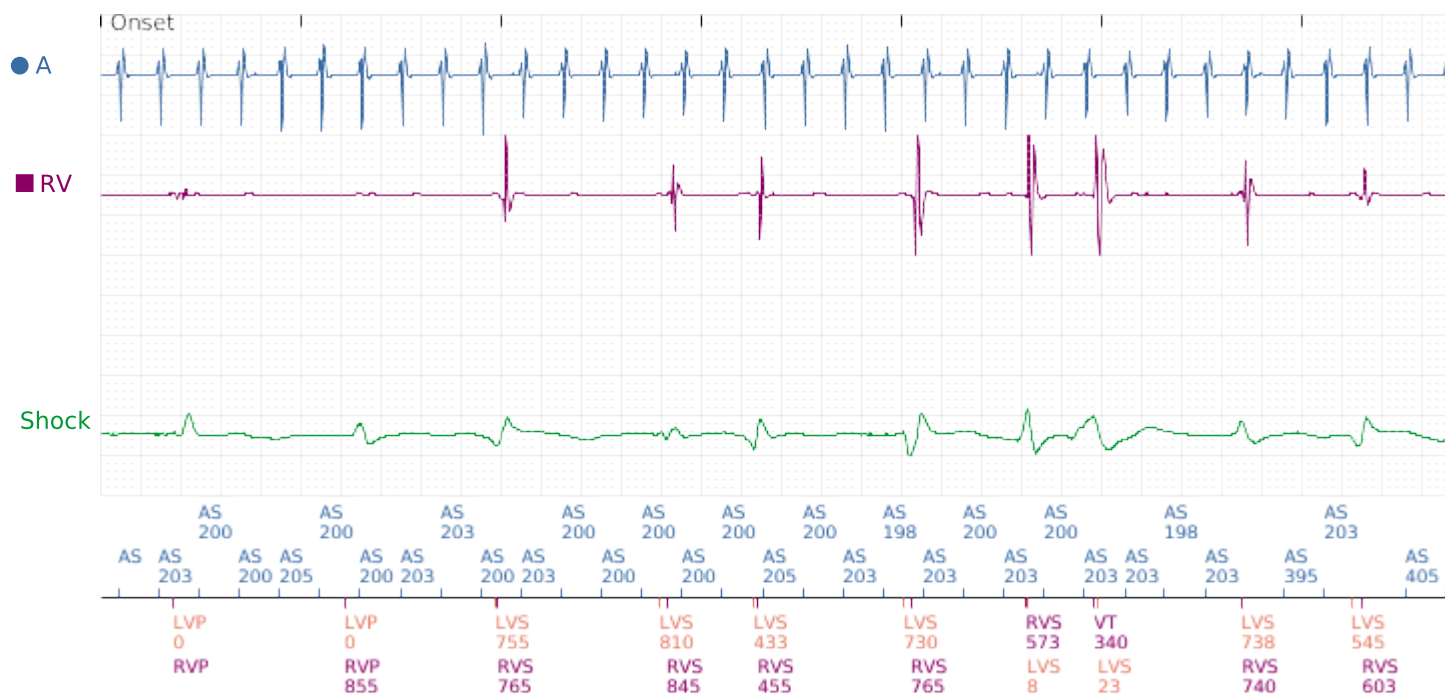

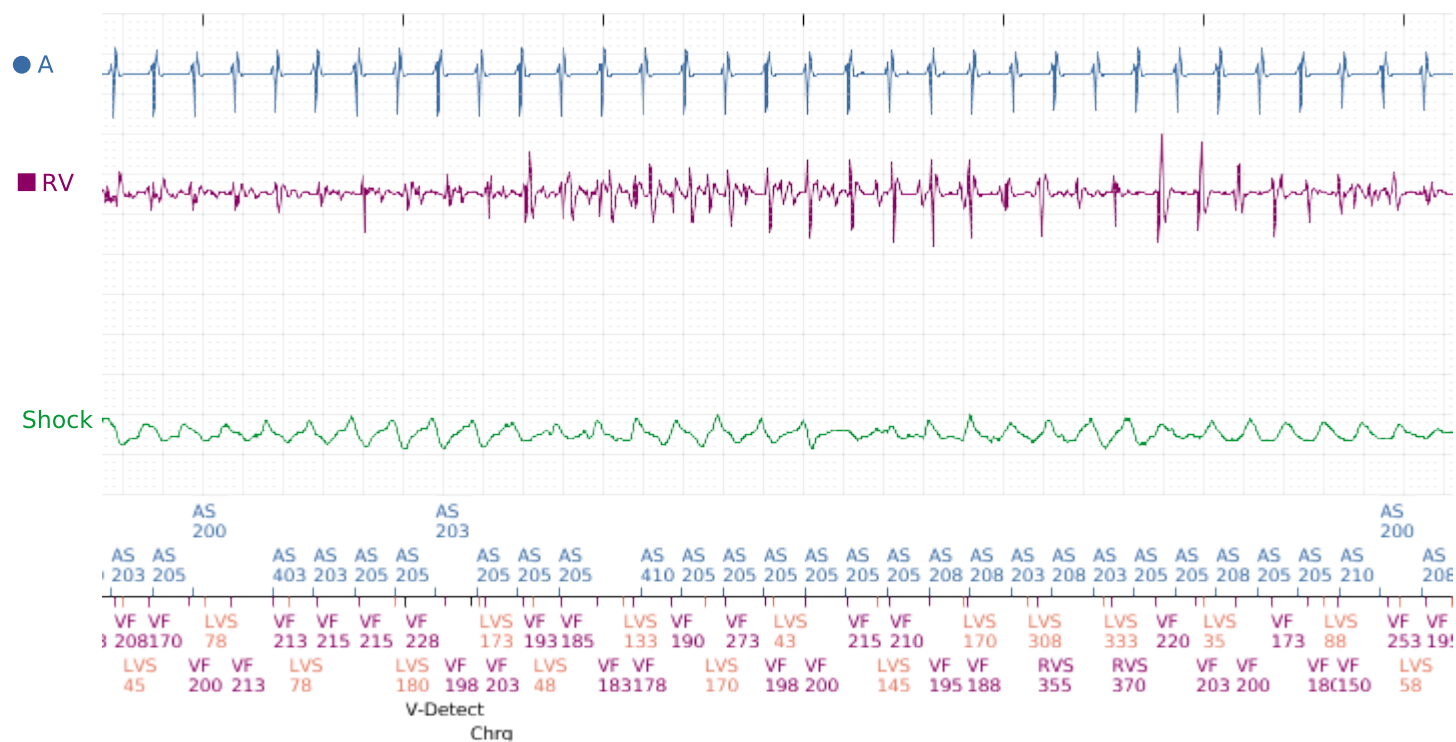



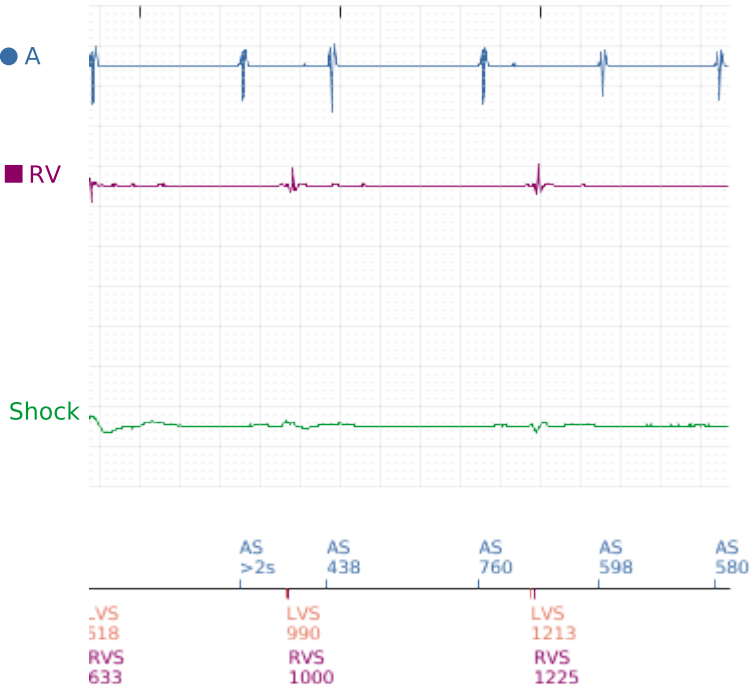

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

