



Date of Birth:
Device: **RESONATE EL ICD D432**
Clinic:
Search Tags:
Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **26 Jan 2023 03:11 CET**
Last Office Interrogation: **06 Dec 2022**
Implant Date:
Patient Group:

V-149: 18 Dec 2022 09:37, VT-1, V Rate: 148 min⁻¹

Detail

VT-1 Event Onset

Avg V Rate	148 min ⁻¹
Detection	Rhythm ID
Template	18 Dec 2022 09:26
RhythmMatch™ Threshold	94 %

At V-Detect

Avg V Rate	150 min ⁻¹
Rate Zone	VT-1
RhythmID Correlated	True
RhythmMatch™	98 %
SRD Met	(False, Off)
ATP Timeout	False

Attempt 1, Non Therapy V

Elapsed Time 00:00:10



Attempt Information



Tachy therapy is programmed off.

Event Ended 00:00:34

EGM displayed at 25mm per second



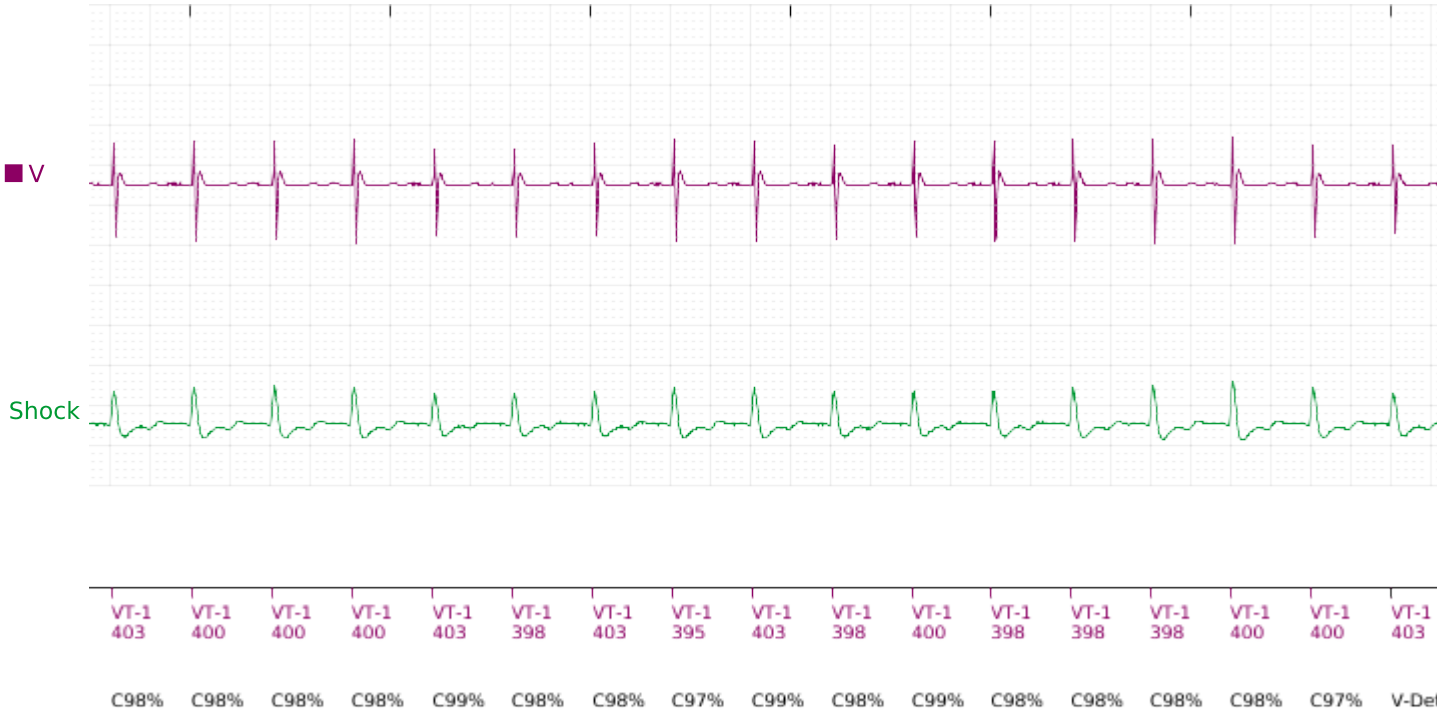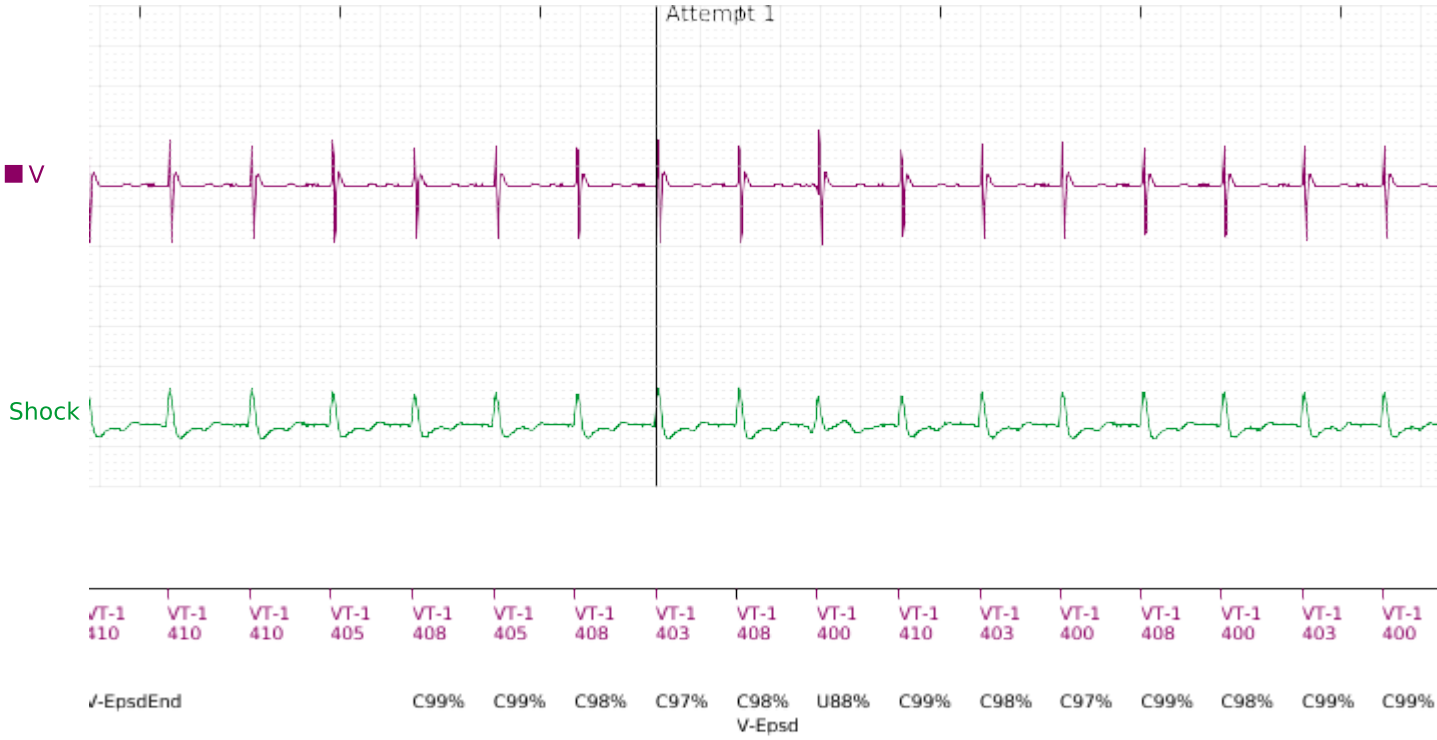

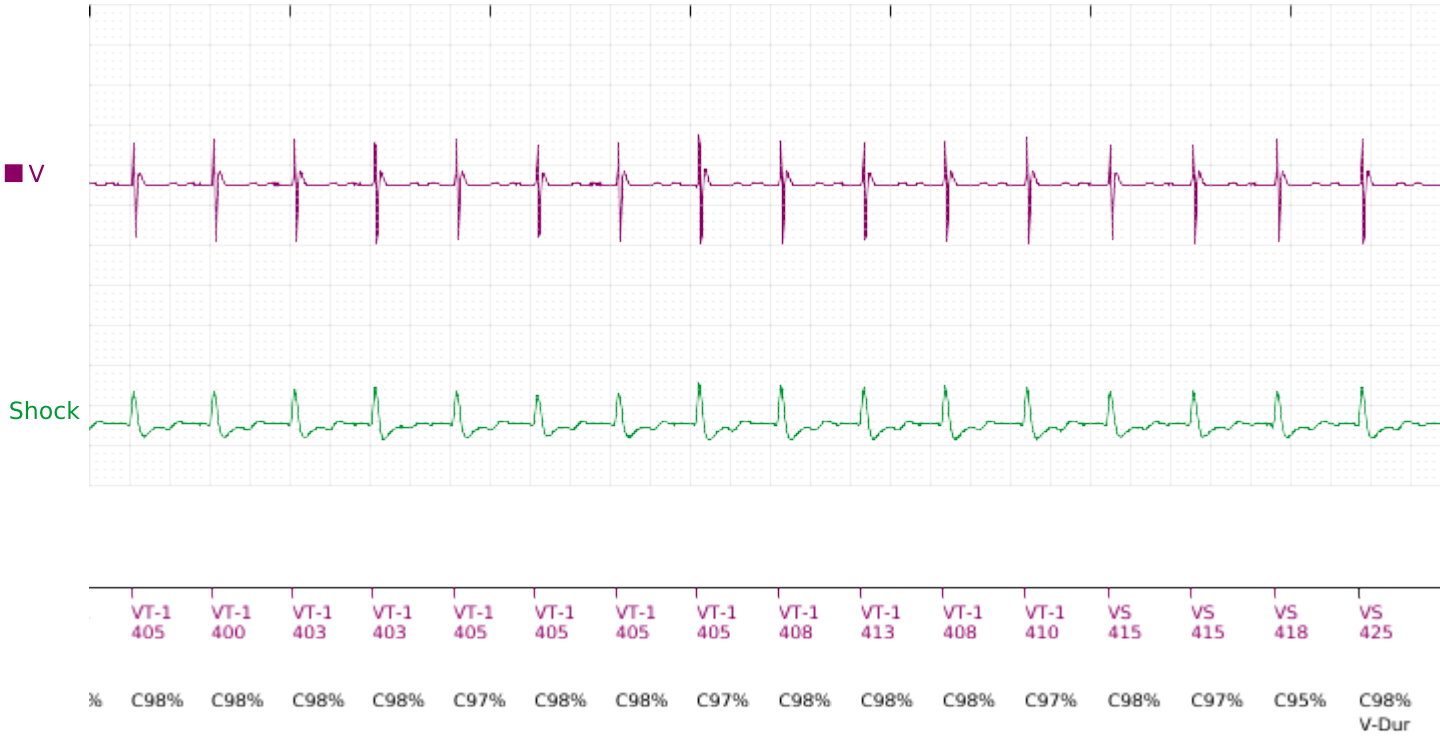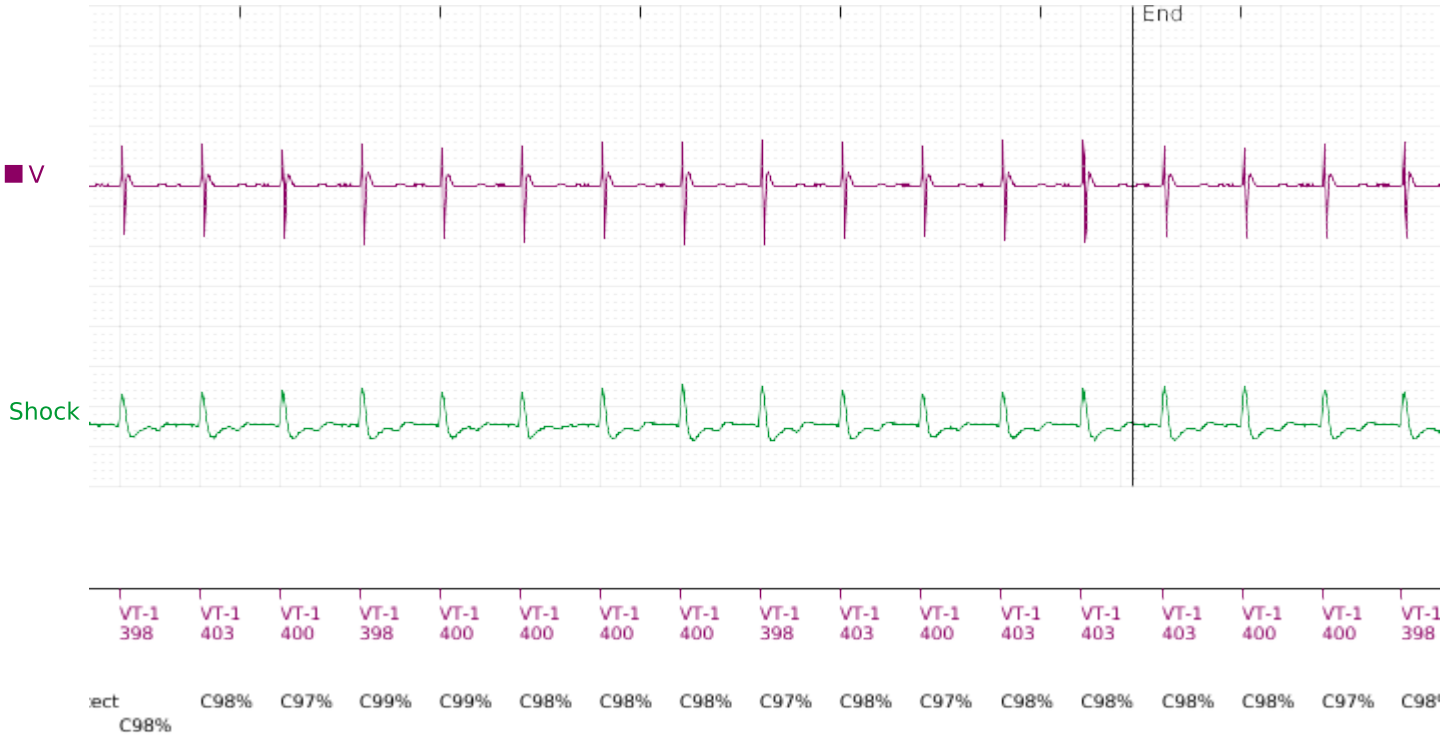

■ V



VS	VS	VS	VS	VS	VS	VS	VS	VS	VS	VS	VS	VS	VS	VS	VS
435	435	435	435	438	440	435	438	435	435	440	435	435	435	433	440
C98%	C98%	C98%	C98%	C97%	C98%	C98%	C97%	C98%	C98%	C97%	C99%	C99%	C98%	C98%	C98

■ V



	VS	VS	VS	VS	VS	
	438	445	435	440	443	453
%	C98%	C98%	C98%	C99%	C99%	C98%

