



Date of Birth:
Device: **RESONATE X4 CRT-D**

Latest Device Transmission: **14 Oct 2022 00:11 CEST**

Last Office Interrogation: **06 Oct 2022**

Clinic:
Search Tags:
Tachy Mode: **Monitor + Therapy**

Implant Date:
Patient Group:

V-17: 20 Sep 2022 10:20, VT, A Rate: 55 min⁻¹, V Rate: 162 min⁻¹

Detail

VT Event Onset

Avg A Rate 55 min⁻¹
Avg V Rate 162 min⁻¹
Detection Rhythm ID
Template 18 Sep 2022 03:01
RhythmMatch™ Threshold 94 %

At V-Detect

Avg A Rate 62 min⁻¹
Avg V Rate 156 min⁻¹
Rate Zone VT
Stability 4 ms
V>A Rate True
AFib False
RhythmID Correlated False
RhythmMatch™ 77 %
SRD Met (False, Off)
ATP Timeout False


Attempt 1, Burst V ATP


Elapsed Time 00:00:15
ATP Information
Number of Bursts 1


Event Ended


00:00:30

EGM displayed at 25mm per second

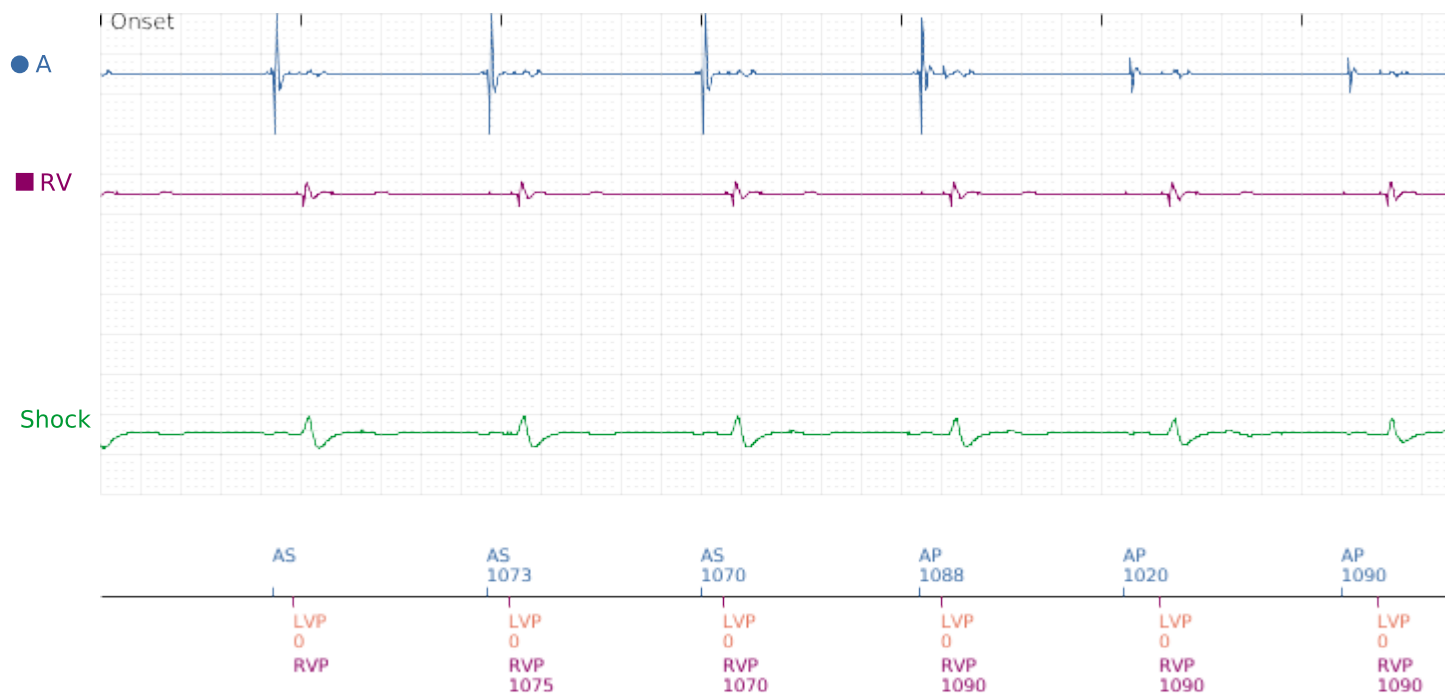

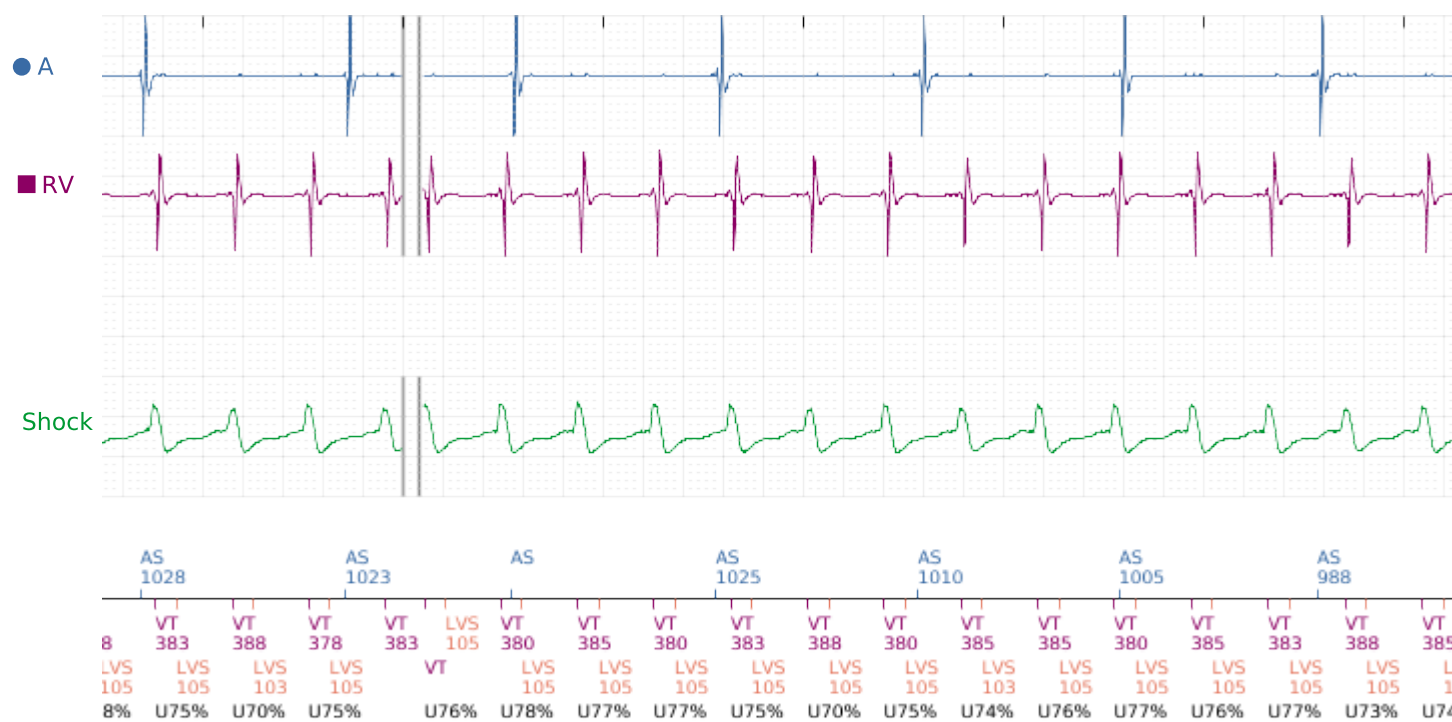

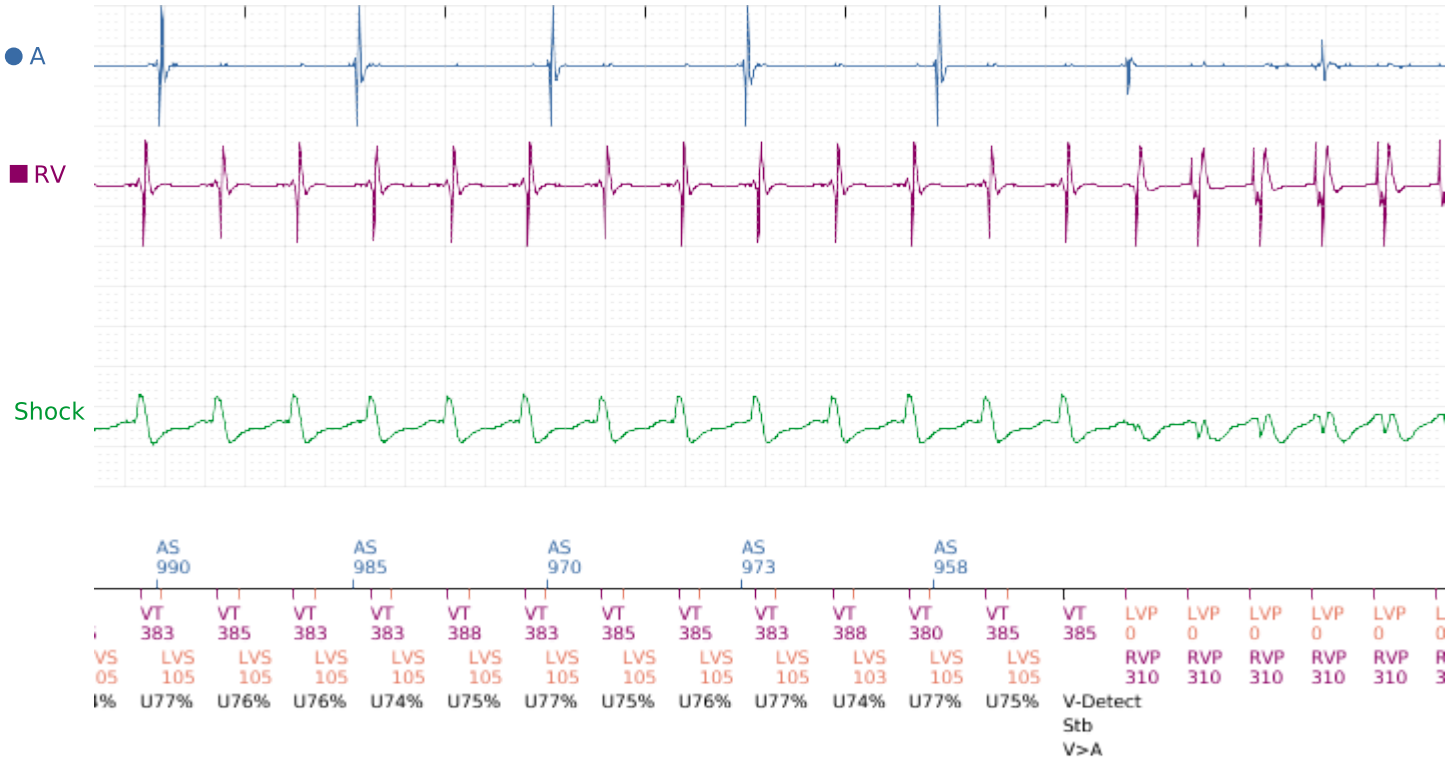

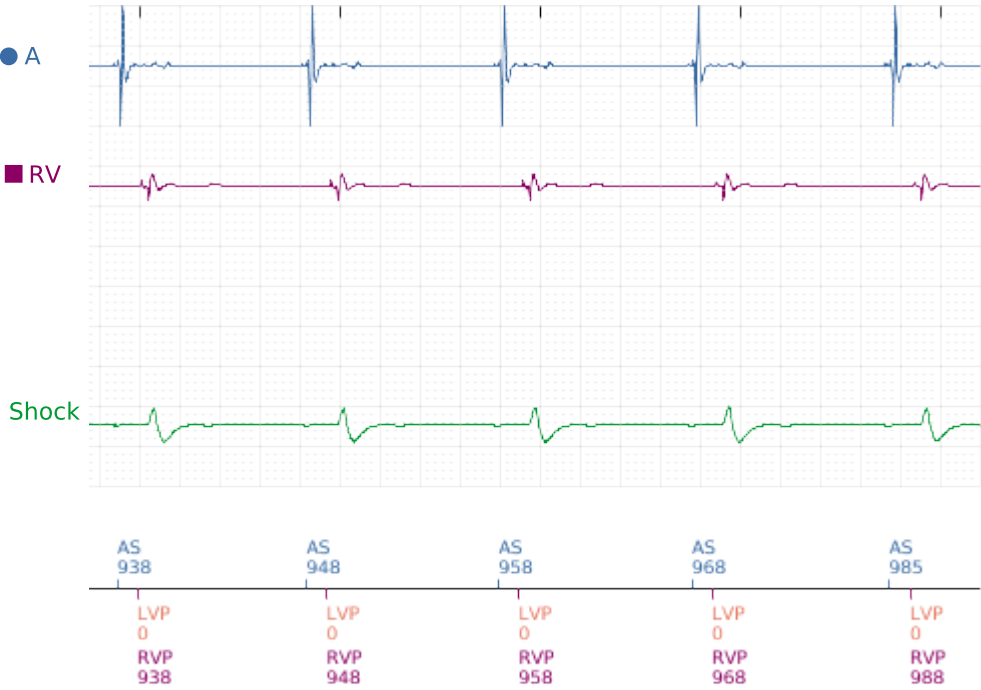

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	○ A Pace

