



Date of Birth:
 Device: **AUTOGEN EL ICD D176**
 Clinic:
 Search Tags:
 Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **26 Dec 2022 07:01 CET**
 Last Office Interrogation: **30 Aug 2022**
 Implant Date:
 Patient Group:

V-415: 05 Mar 2022 12:29, VT-1, A Rate: 161 min⁻¹, V Rate: 161 min⁻¹

Detail

VT-1 Event Onset

Avg A Rate 161 min⁻¹
 Avg V Rate 161 min⁻¹
 Detection Rhythm ID
 Template 02 Mar 2022 03:23
 RhythmMatch™ Threshold 94 %

At V-Detect

Avg A Rate 159 min⁻¹
 Avg V Rate 159 min⁻¹
 Rate Zone VT-1
 Stability (4 ms, Off)
 V>A Rate (False, Off)
 AFib (False, Off)
 RhythmID Correlated True
 RhythmMatch™ 98 %
 SRD Met (False, Off)
 ATP Timeout False

Attempt 1, Non Therapy V

Elapsed Time 00:00:12


Attempt Information



Tachy therapy is programmed off.



Event Ended

00:00:23

EGM displayed at 25mm per second

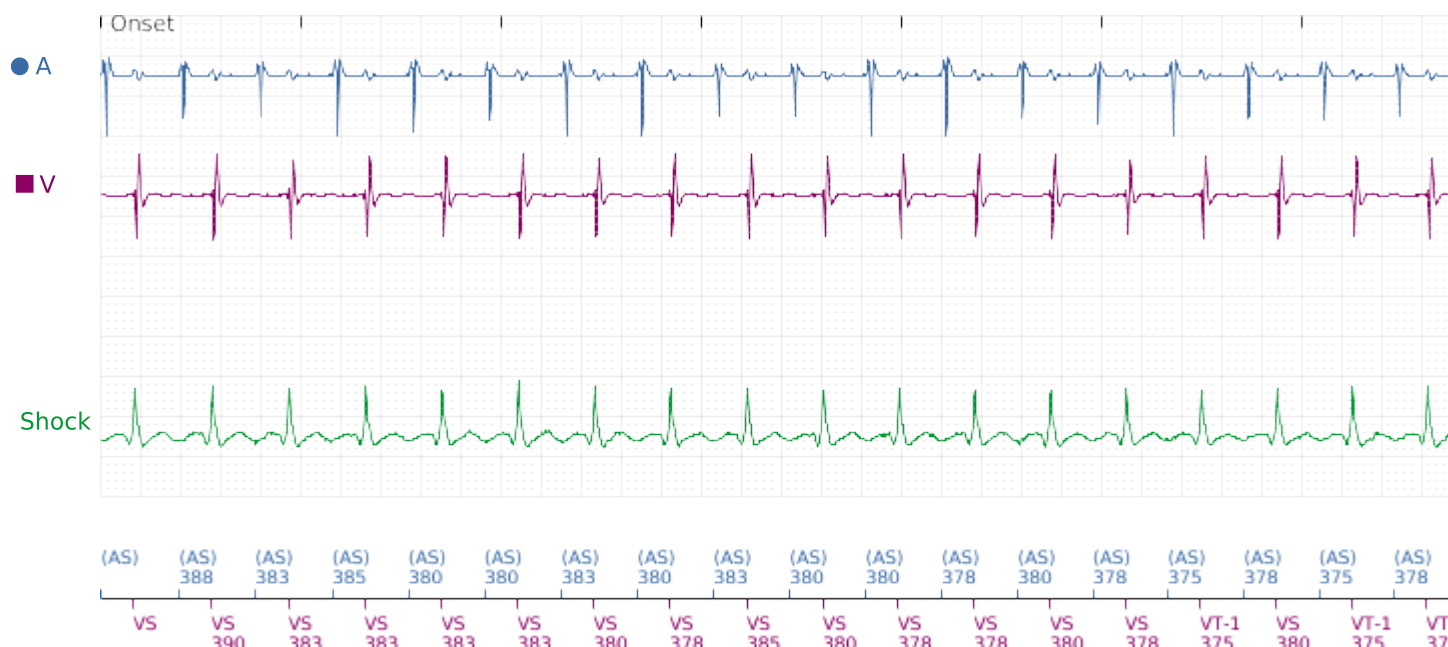

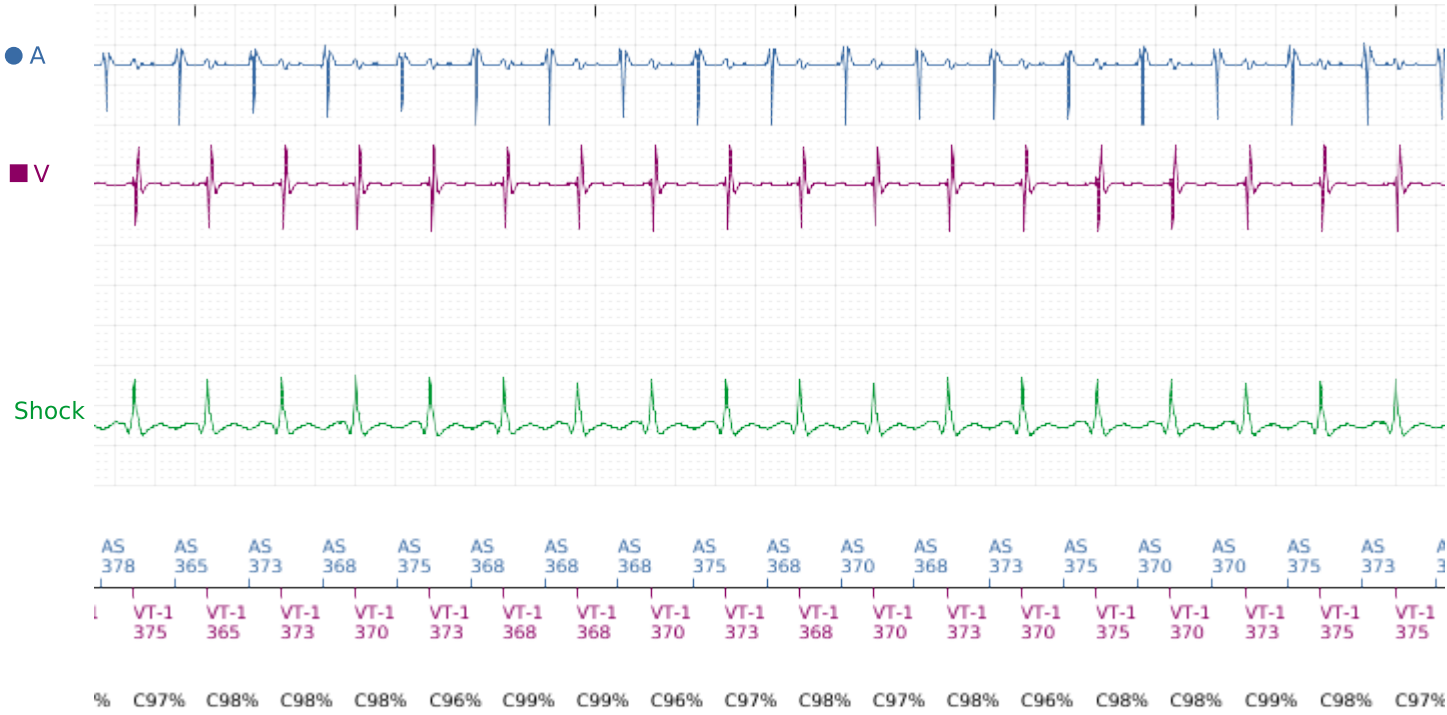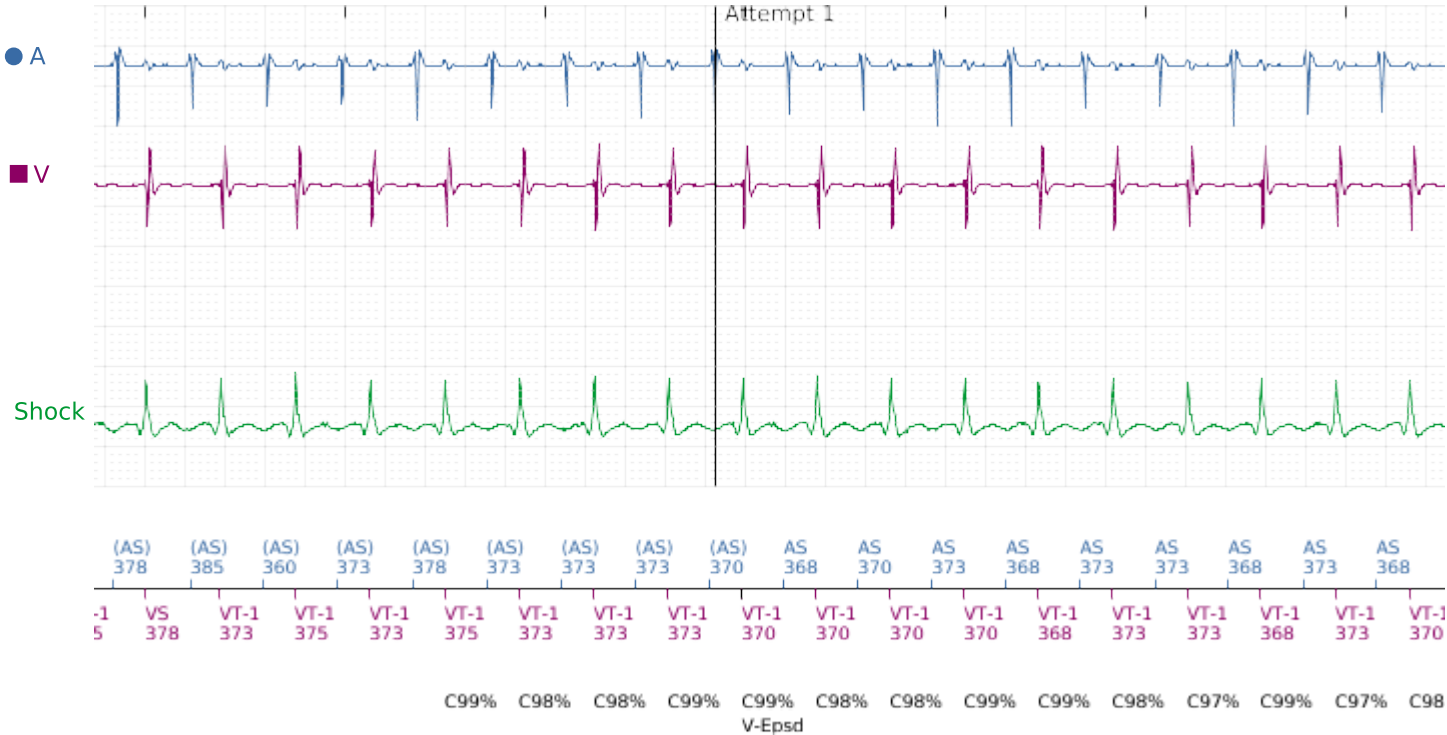

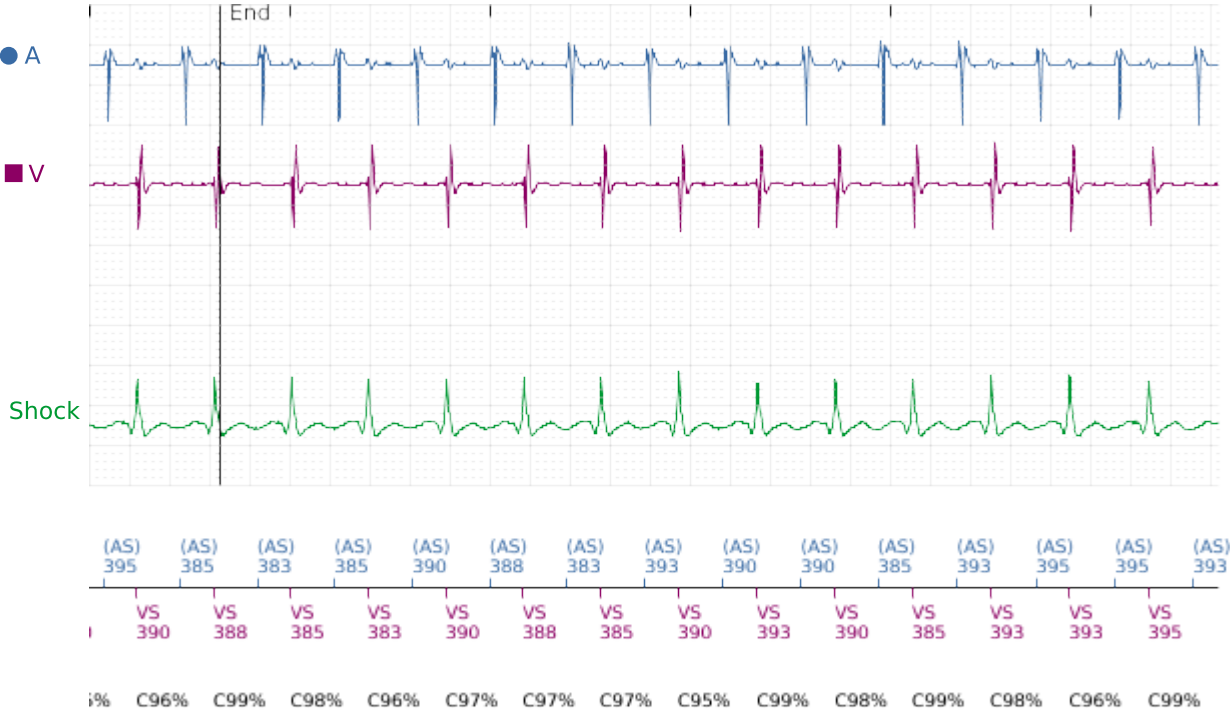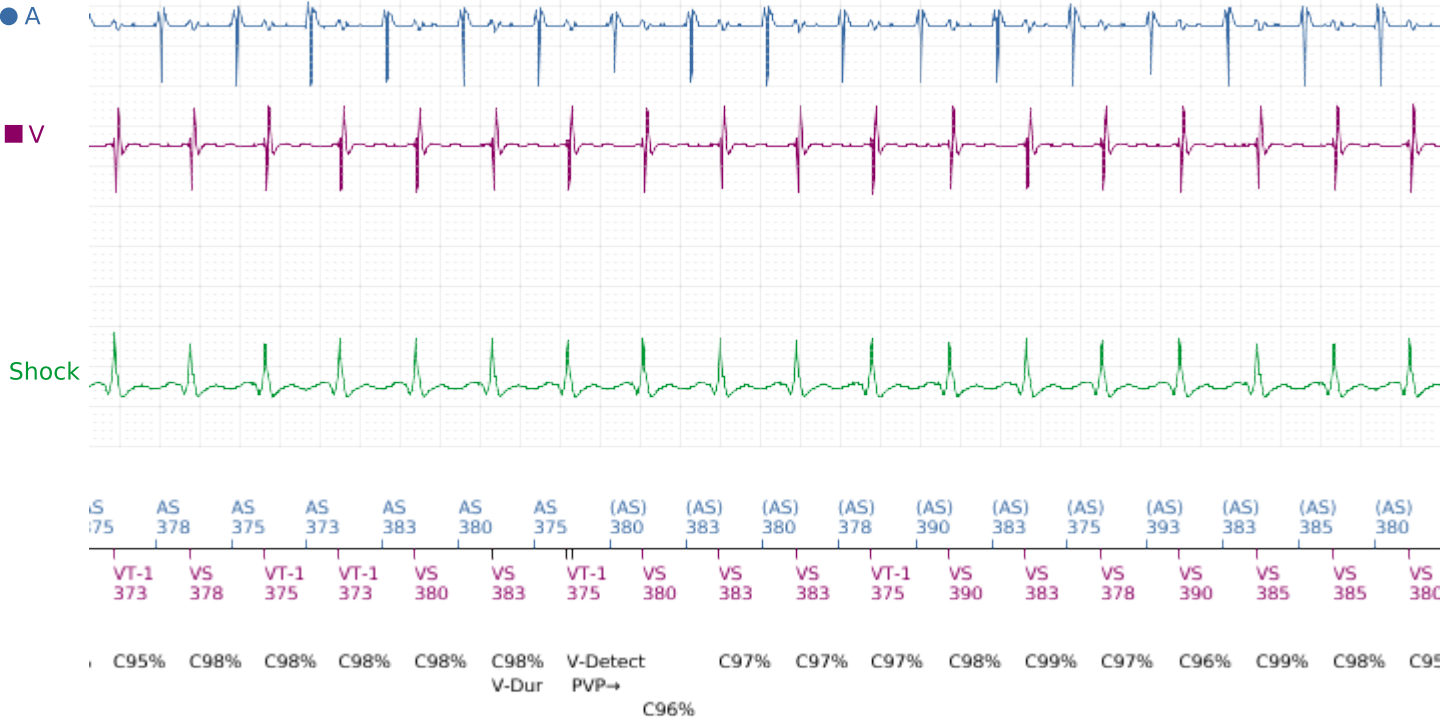

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

