



Date of Birth:
 Device: **AUTOGEN X4 CRT-D G179**
 Clinic:
 Search Tags:
 Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **26 Dec 2022 01:41 CET**
 Last Office Interrogation: **10 Feb 2022**
 Implant Date:
 Patient Group:

V-19: 08 Sep 2018 06:08, VT, A Rate: 181 min⁻¹, V Rate: 181 min⁻¹

Detail

VT Event Onset

Avg A Rate	181 min ⁻¹
Avg V Rate	181 min ⁻¹
Detection	Onset/Stability
Onset	Percent
Template	N/R

At V-Detect

Avg A Rate	181 min ⁻¹
Avg V Rate	181 min ⁻¹
Rate Zone	VT
Stability	2 ms
V>A Rate	False
AFib	True
RhythmMatch™	N/R
SRD Met	(False, Off)
ATP Timeout	False
Onset Intvl	(0 ms, Off)
Onset %	0 %

Attempt 1, Burst V ATP



Elapsed Time	00:00:05
ATP Information	
Number of Bursts	1


Event Ended

00:00:18

EGM displayed at 25mm per second



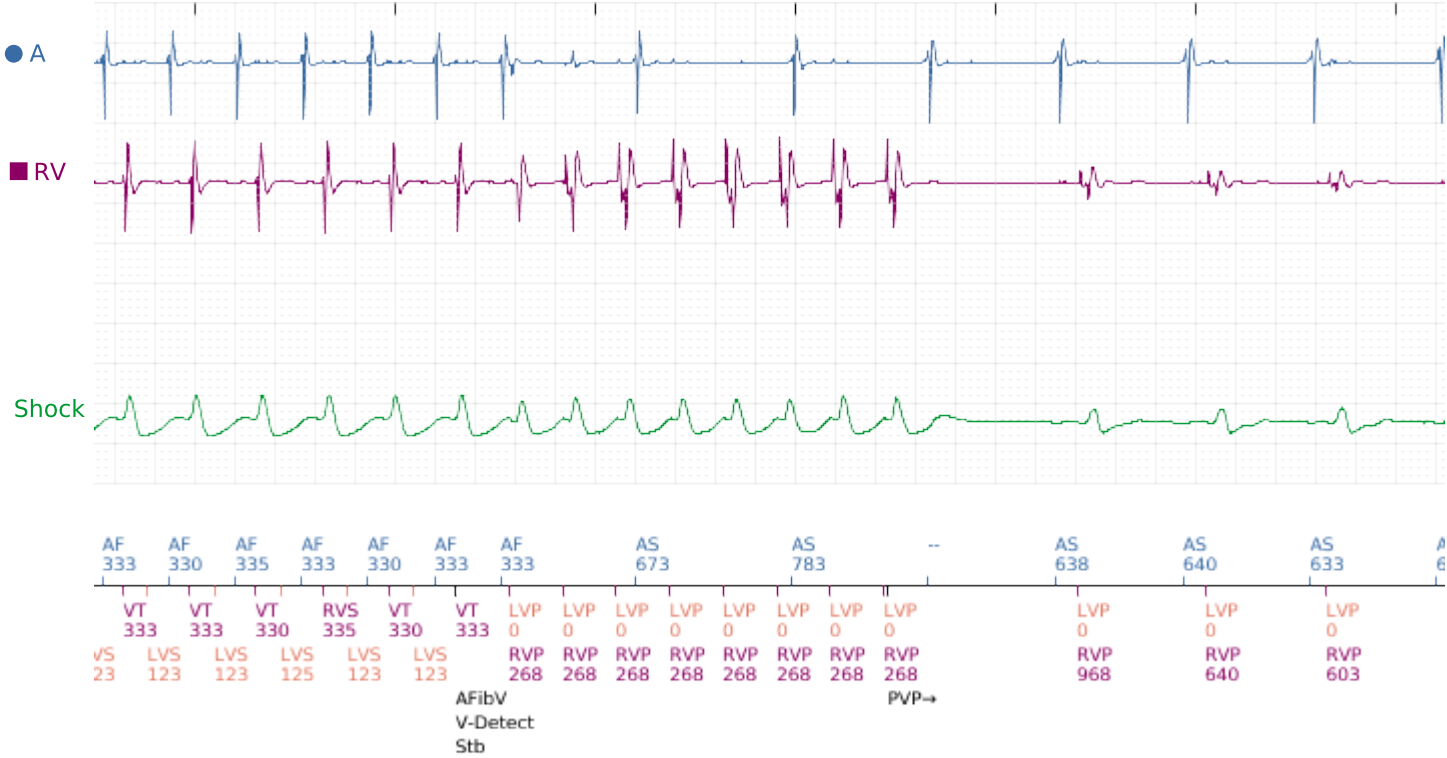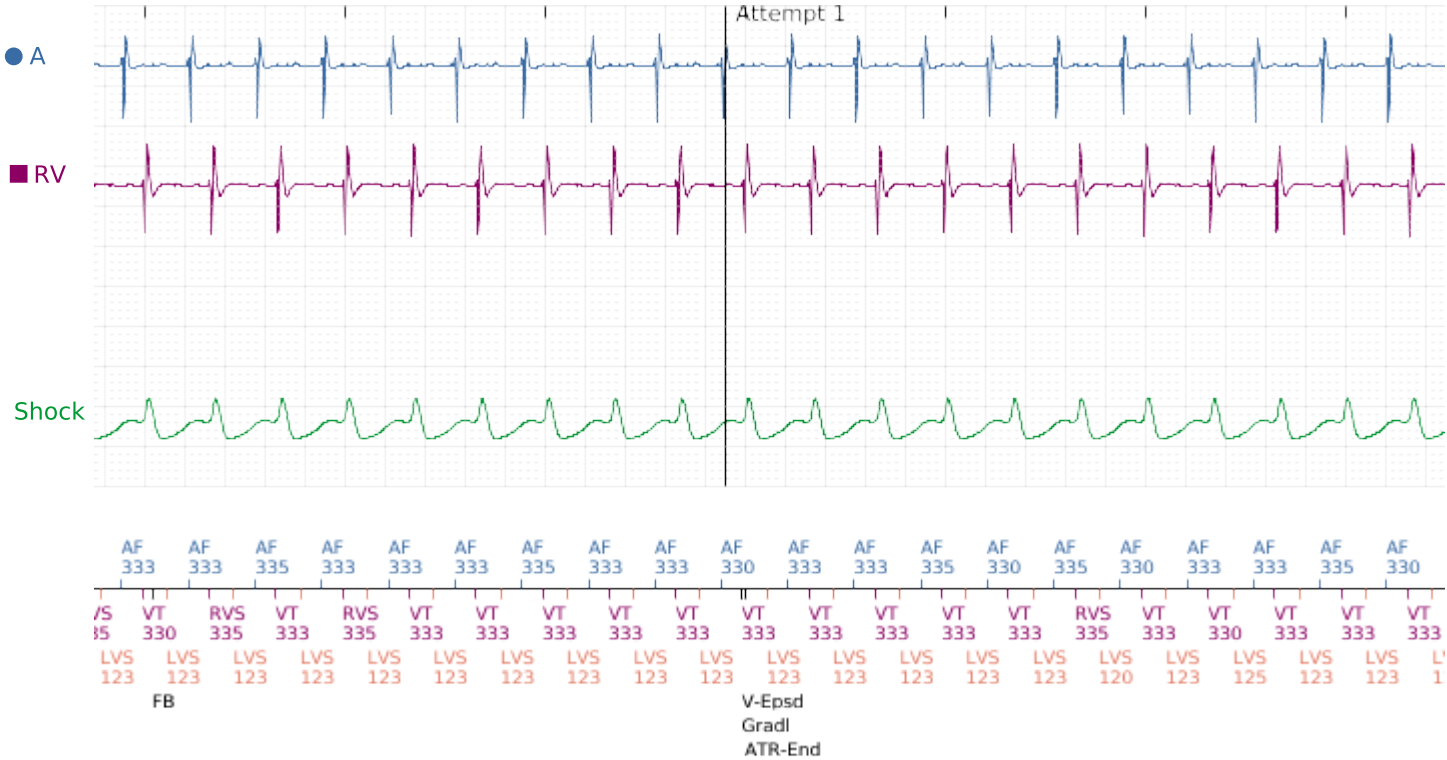

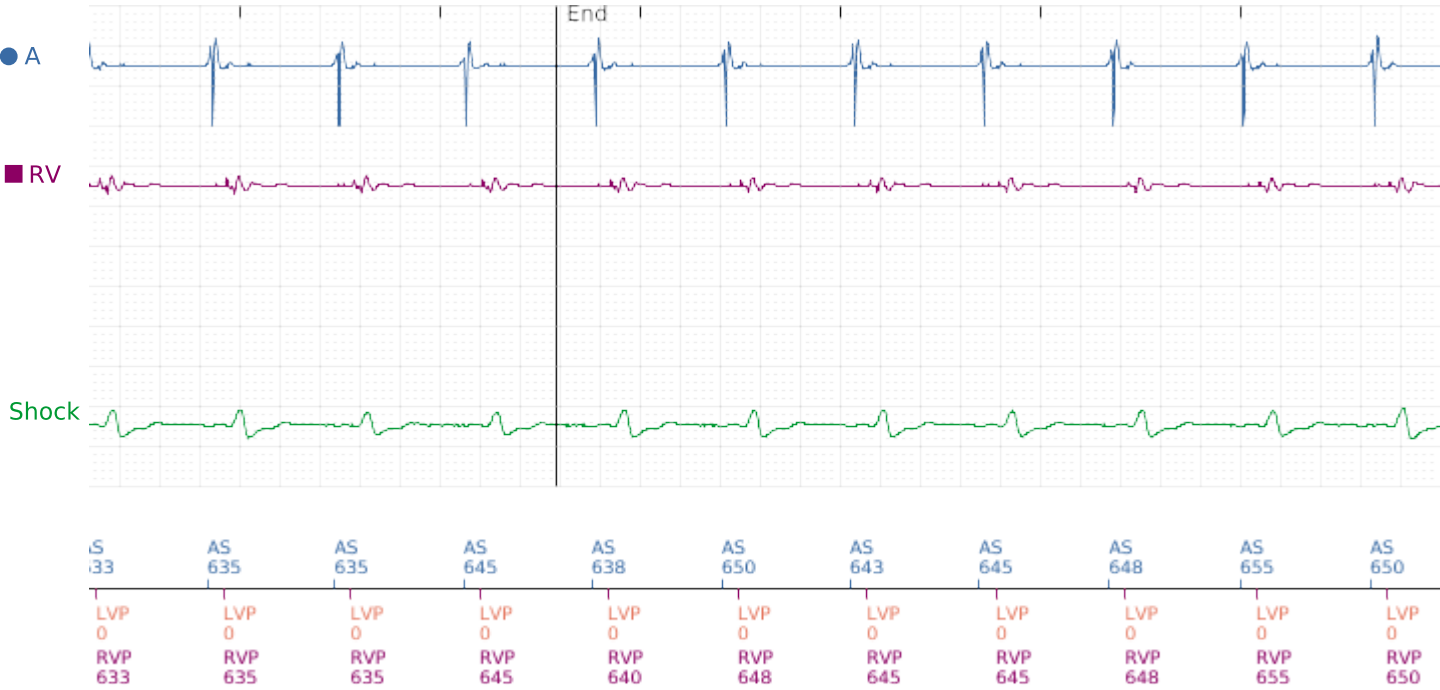

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	○ A Pace

