



Date of Birth:
 Device: **AUTOGEN X4 CRT-D G179**
 Clinic:
 Search Tags:
 Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **19 Dec 2022 03:01 CET**
 Last Office Interrogation: **14 Nov 2022**
 Implant Date:
 Patient Group:

V-16: 29 Apr 2021 08:43, VF, A Rate: 30 min⁻¹, V Rate: 264 min⁻¹

Detail

VF Event Onset

Avg A Rate 30 min⁻¹
 Avg V Rate 264 min⁻¹
 Detection Rate Only
 Template N/R

At V-Detect

Avg A Rate 30 min⁻¹
 Avg V Rate 311 min⁻¹
 Rate Zone VF
 Stability (45 ms, Off)
 V>A Rate (True, Off)
 AFib (False, Off)
 RhythmMatch™ N/R
 SRD Met (False, Off)
 ATP Timeout False
 Onset Intvl (330 ms, Off)
 Onset % (44 %, Off)


Attempt 1, 41 J V Shock



Elapsed Time 00:00:03
 Shock Information
 Charge Time 10.0 s
 Lead Impedance 67 Ω
 Lead Polarity Initial


Event Ended

00:00:46

EGM displayed at 25mm per second

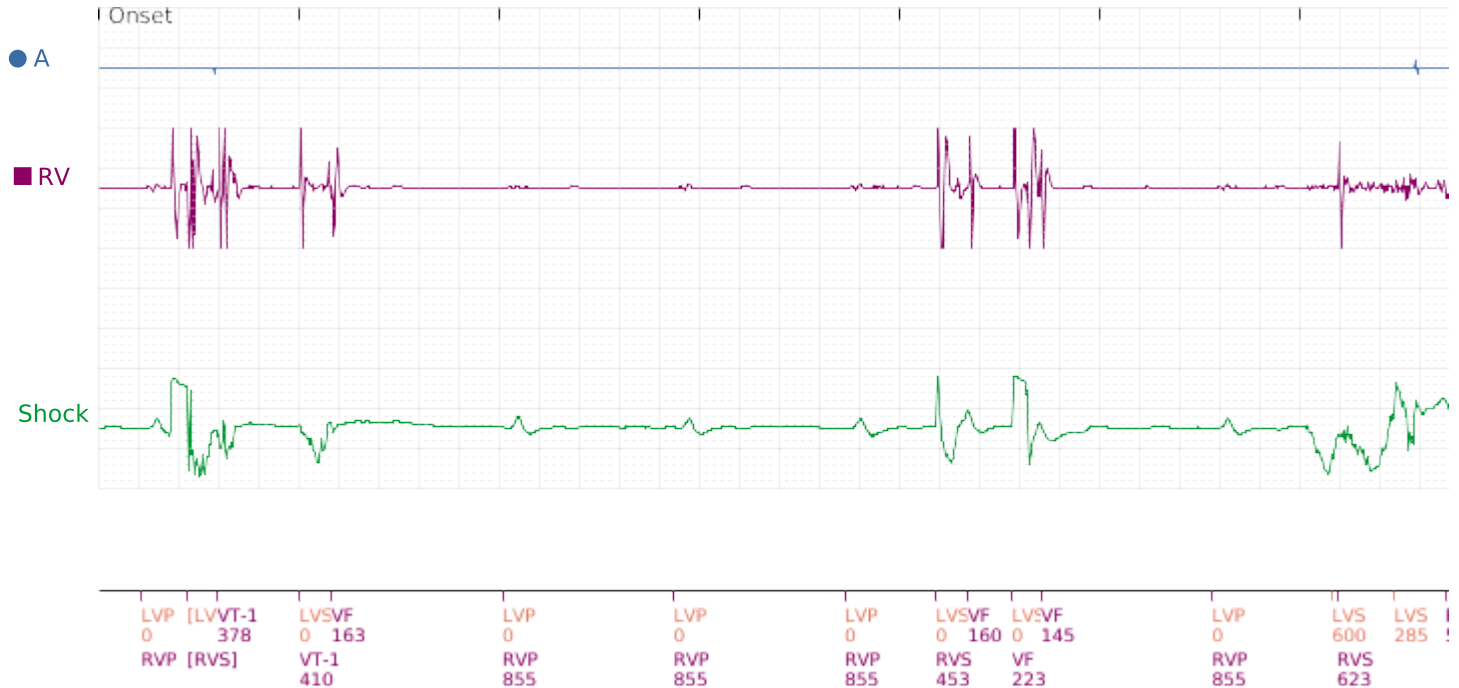

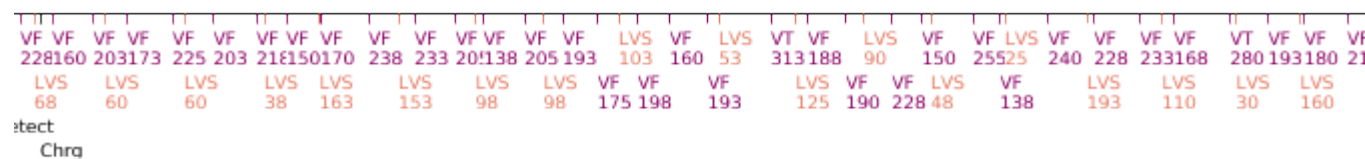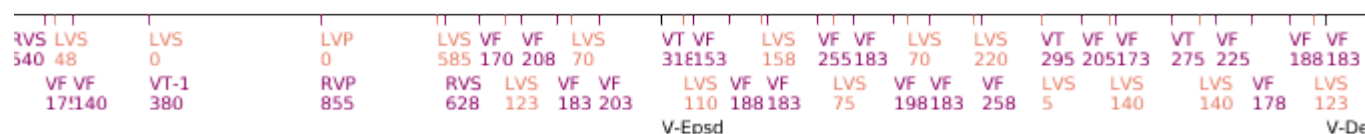

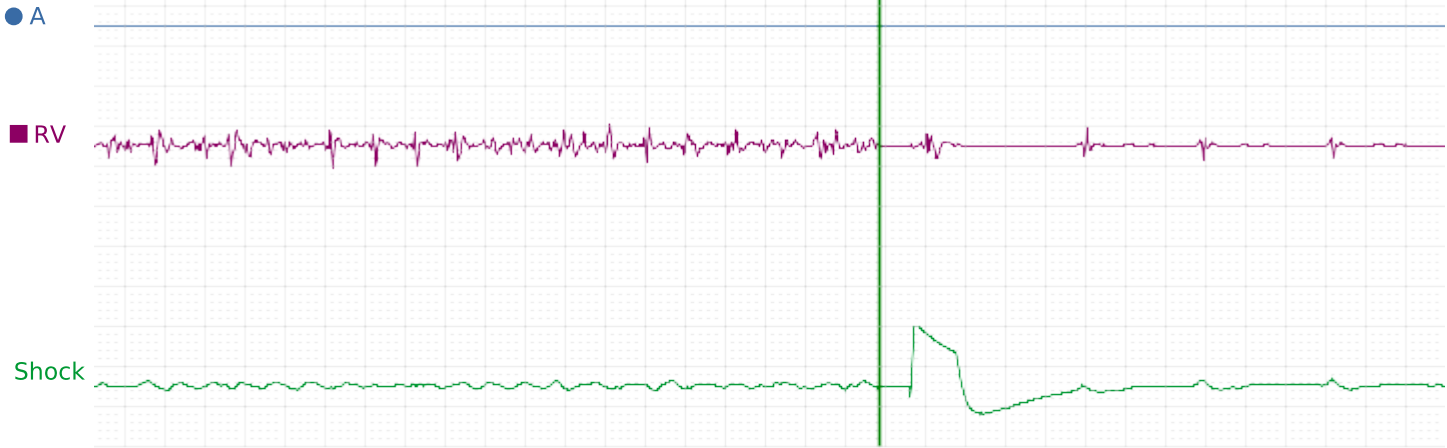

LVS	VF	VF	LVS	LVS	VF	VF	VF	VF	VF	VF	LVS	--	VF	VT	--	RVS	RVS
158	213	260	118	490	218	208	203	188	173	245	95		173	278		590	650
VF	LVS	VF		RVS	LVS	LVS	VF	LVS	VF	VF			LVS			LVS	LVS
153	180	138		493	160	125	158	180	193	190			60			85	88

Chrg 41.0J Shk



LVP	RVS	LVP	LVP	LVP	LVP	LVP	LVP
0	705	0	0	0	0	0	0
RVP	LVS	RVP	RVP	RVP	RVP	RVP	RVP
855	3	855	855	855	855	855	855



↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	○ A Pace

