
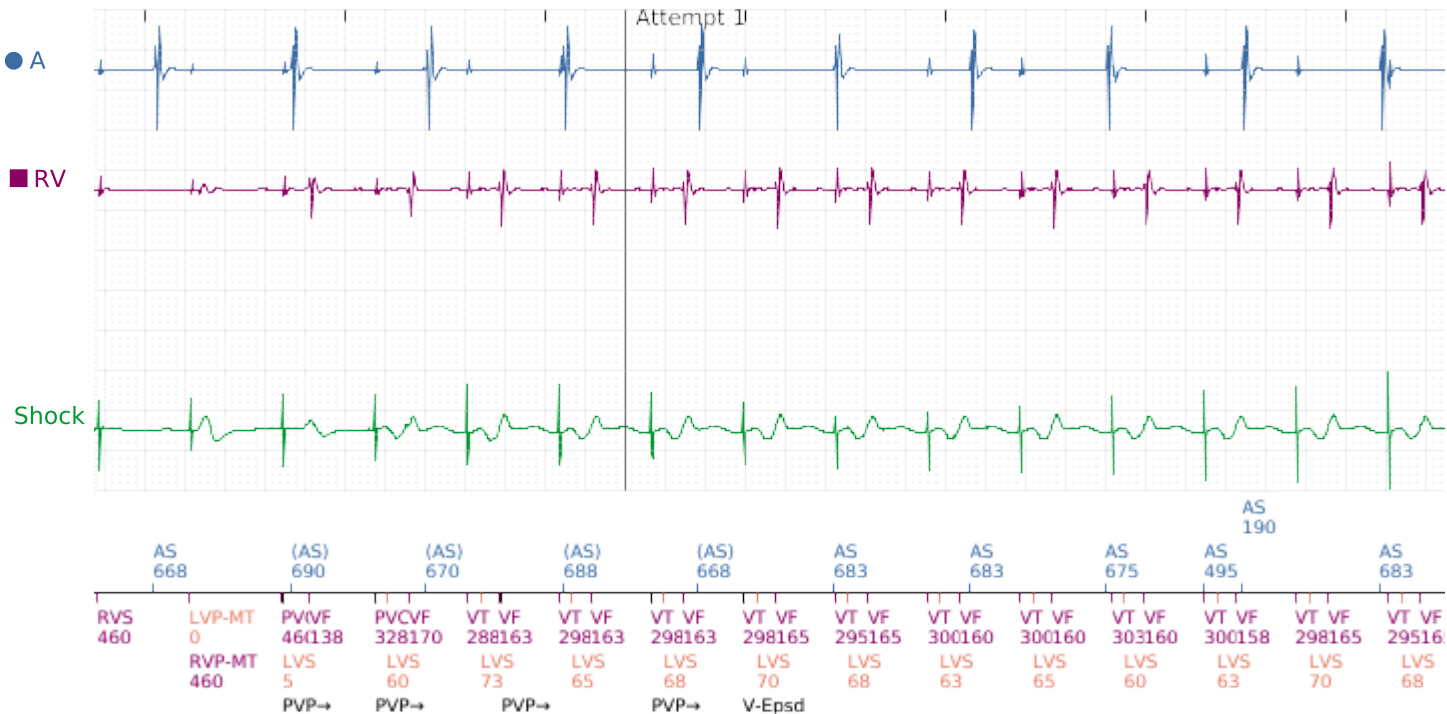



LATITUDE™ Patient Management - Event Detail Report		Report Created: 25 Jan 2023
	Date of Birth:	Latest Device Transmission: 09 Jan 2023 00:52 CET
	Device: RESONATE X4 CRT-D	Last Office Interrogation: 22 Mar 2022
	Clinic:	Implant Date:
	Search Tags:	nt Group:
	Tachy Mode: Monitor + Therapy	


V-1: 29 Apr 2020 13:48, VT, A Rate: 88 min⁻¹, V Rate: 261 min⁻¹


Detail


VT Event Onset			
Avg A Rate	88 min ⁻¹		
Avg V Rate	261 min ⁻¹		
Detection	Rate Only		
Template	N/R		
At V-Detect		Attempt 1, Burst V ATP	
Avg A Rate	116 min ⁻¹	Elapsed Time	00:00:10
Avg V Rate	261 min ⁻¹	ATP Information	
Rate Zone	VT	Number of Bursts	3
Stability	(180 ms, Off)		
V>A Rate	(True, Off)		
AFib	(False, Off)		
RhythmMatch™	N/R		
SRD Met	(False, Off)		
ATP Timeout	False		
Onset Intvl	(159 ms, Off)		
Onset %	(35 %, Off)		
At V-Detect		Attempt 2, Ramp V ATP	
Avg A Rate	119 min ⁻¹	Elapsed Time	00:00:28
Avg V Rate	261 min ⁻¹	ATP Information	
Rate Zone	VT	Number of Bursts	3
ATP Timeout	False		
At V-Detect		Attempt 3, 41 J V Shock	
Avg A Rate	91 min ⁻¹	Elapsed Time	00:00:45
Avg V Rate	261 min ⁻¹	Aborted Attempt	
Rate Zone	VT	No shock attempted due to fail to reconfirm	
ATP Timeout	False		
Event Ended			00:01:11
EGM displayed at 25mm per second			


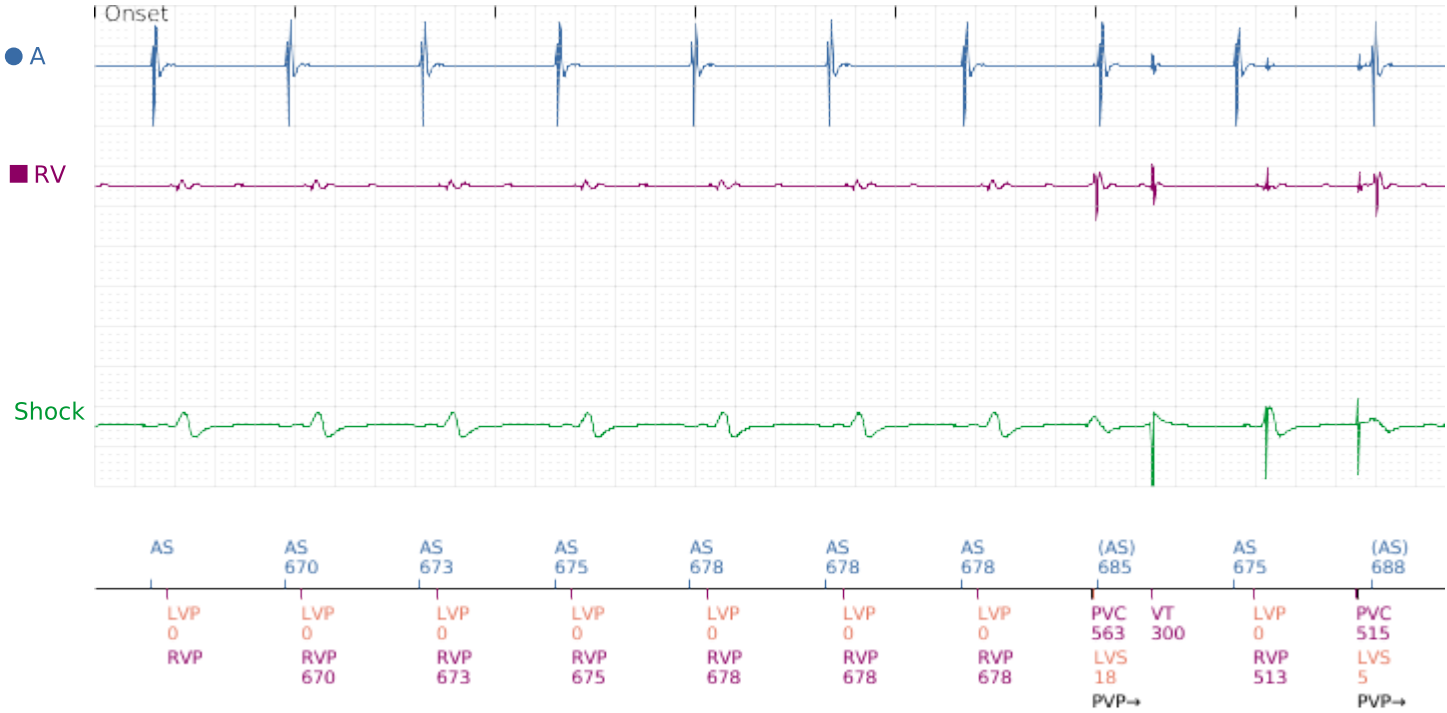


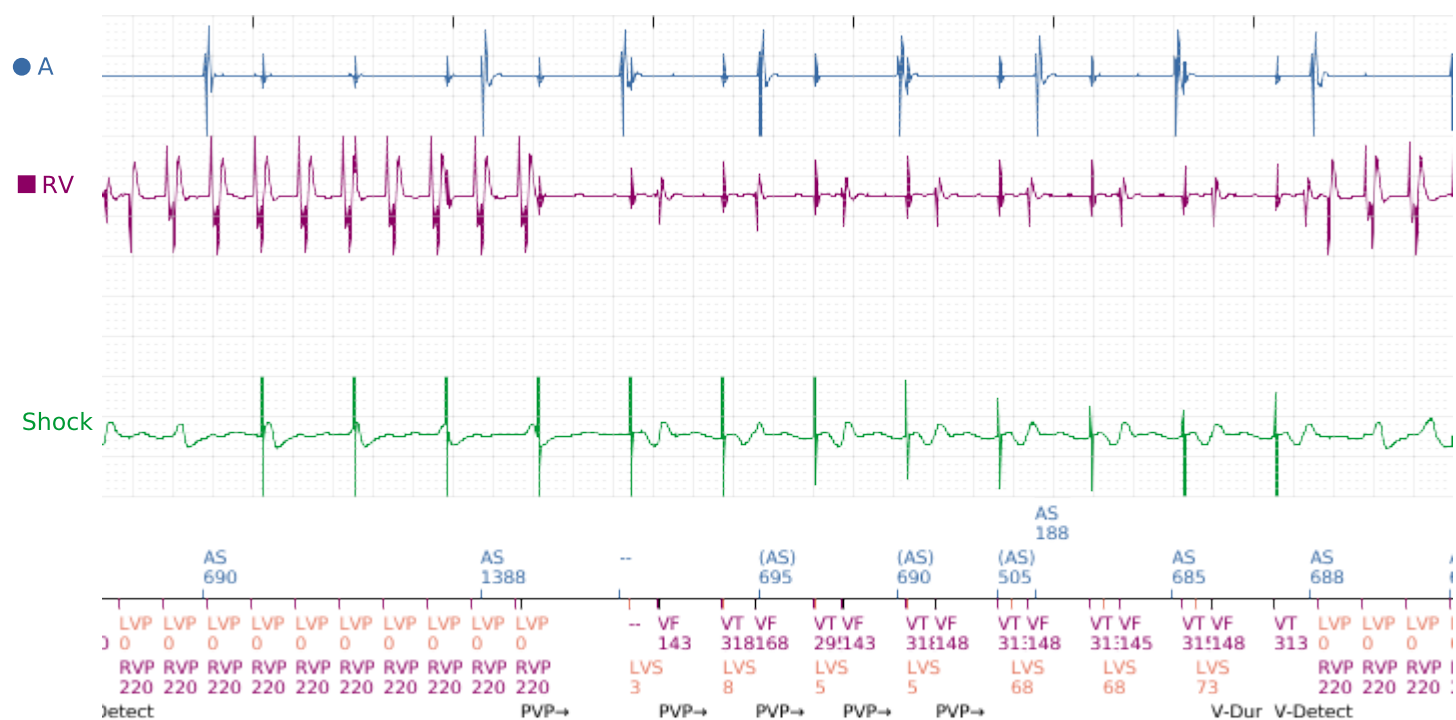

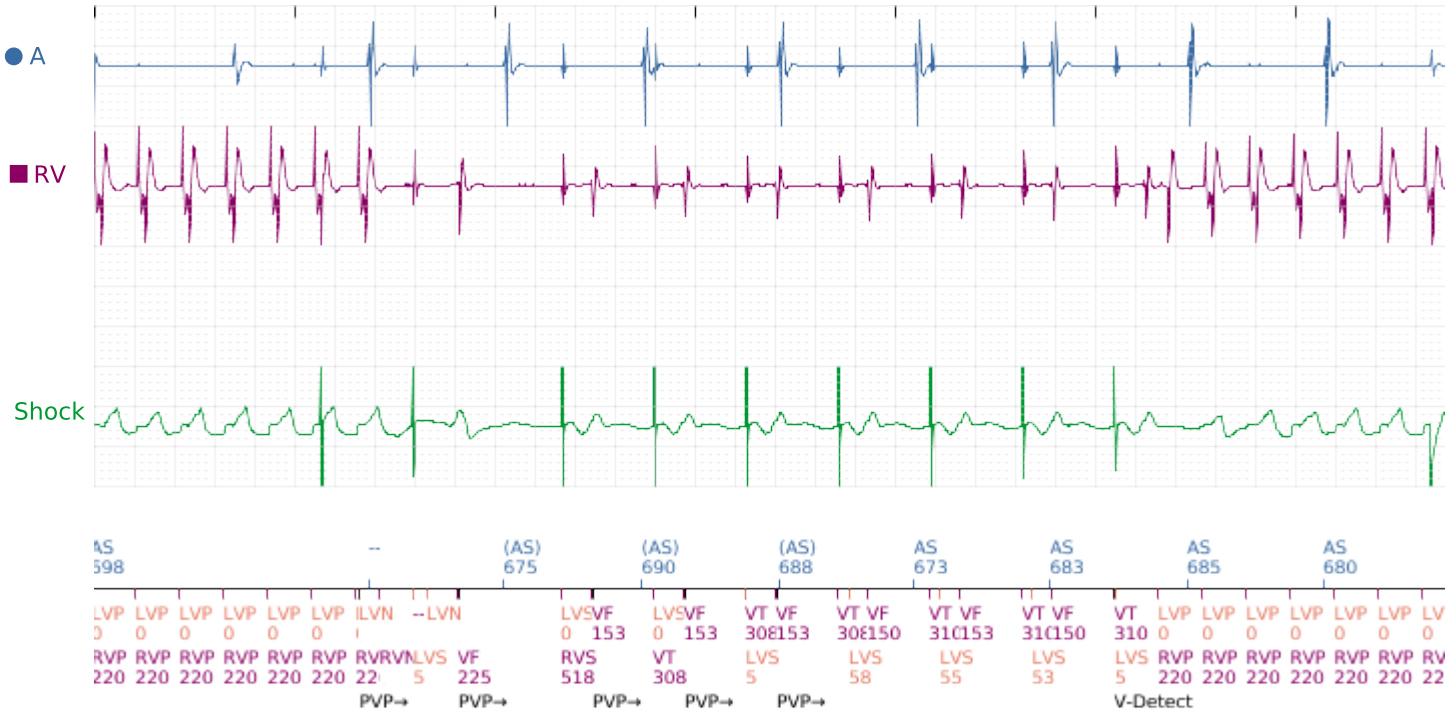

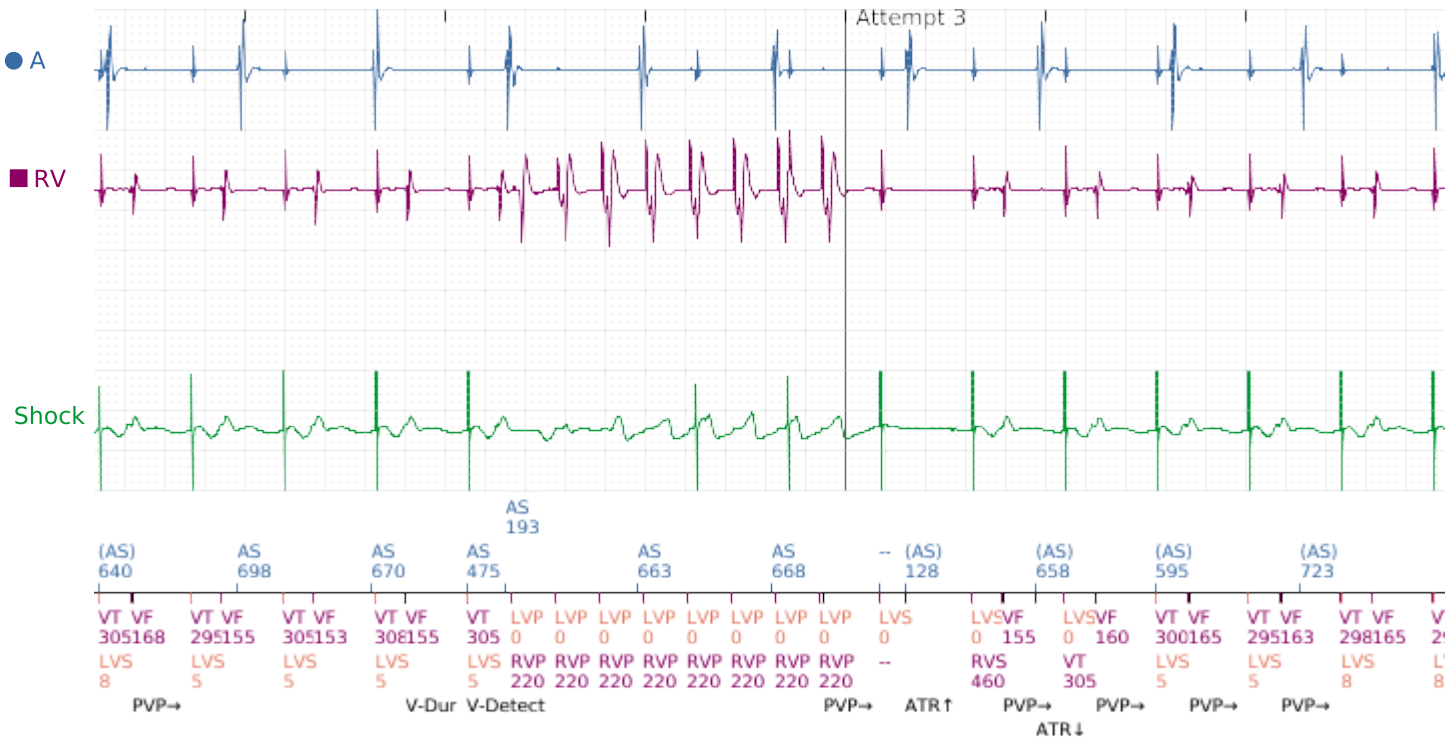

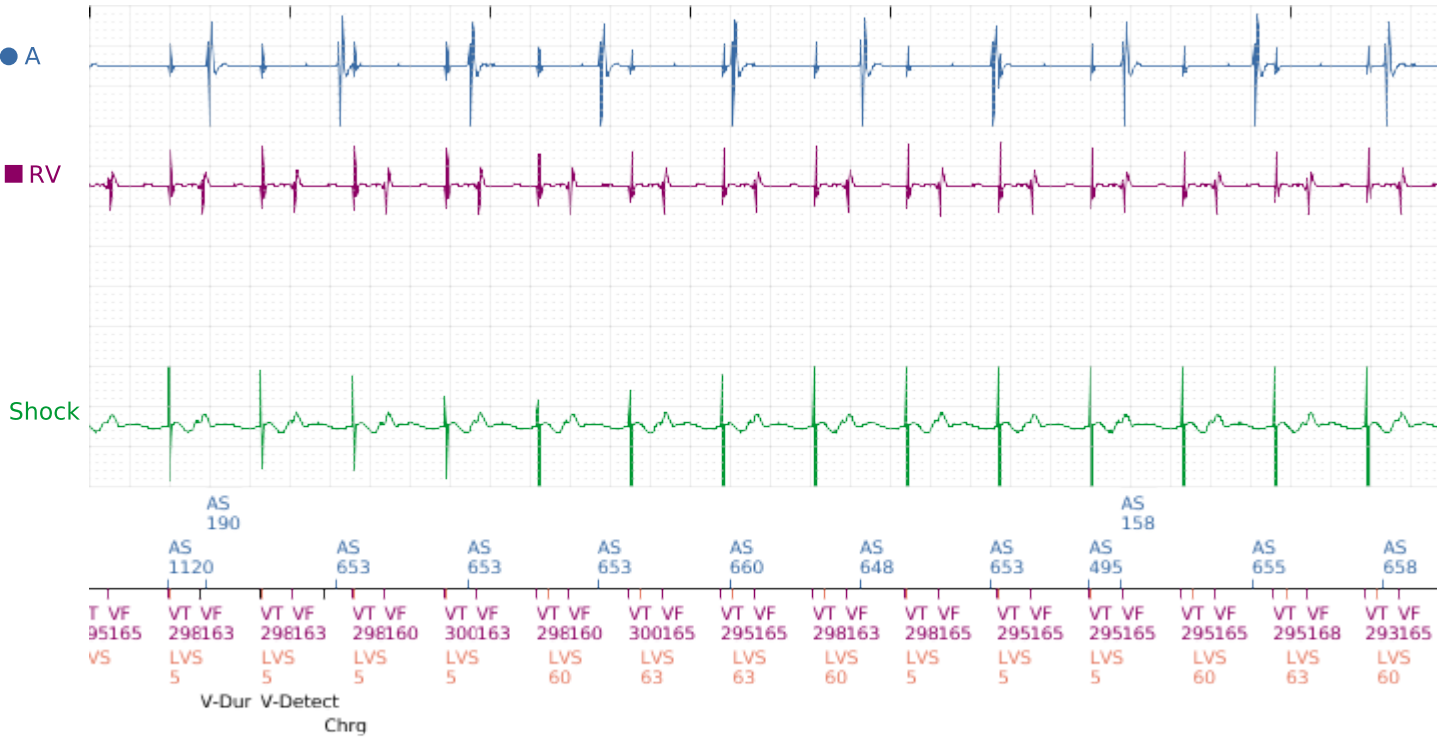

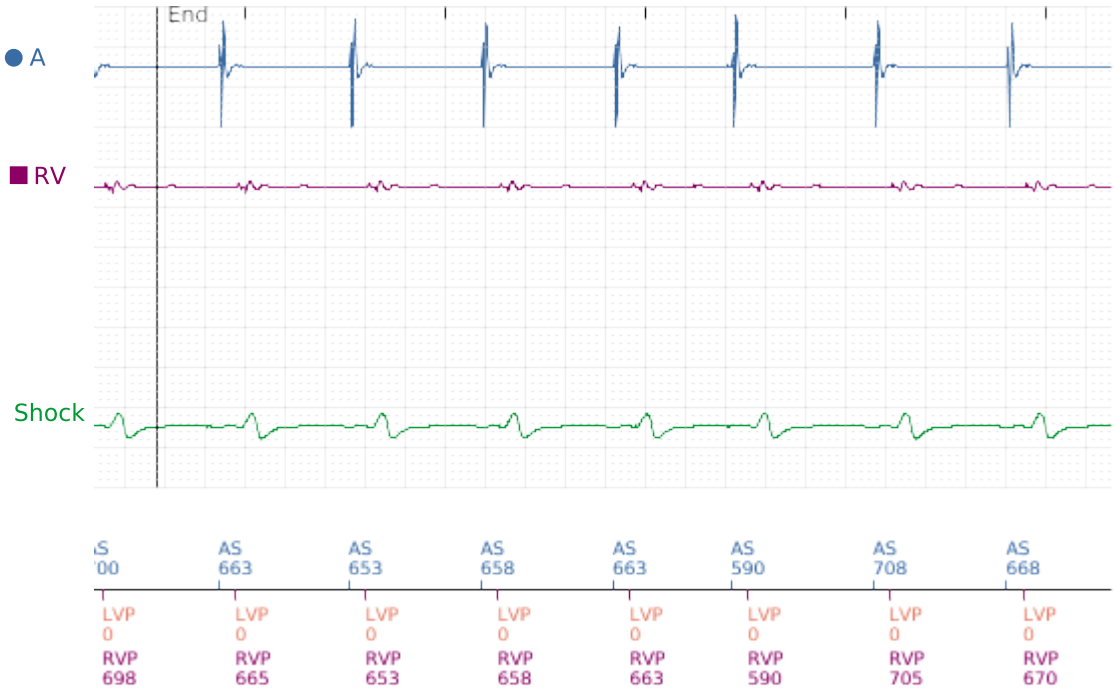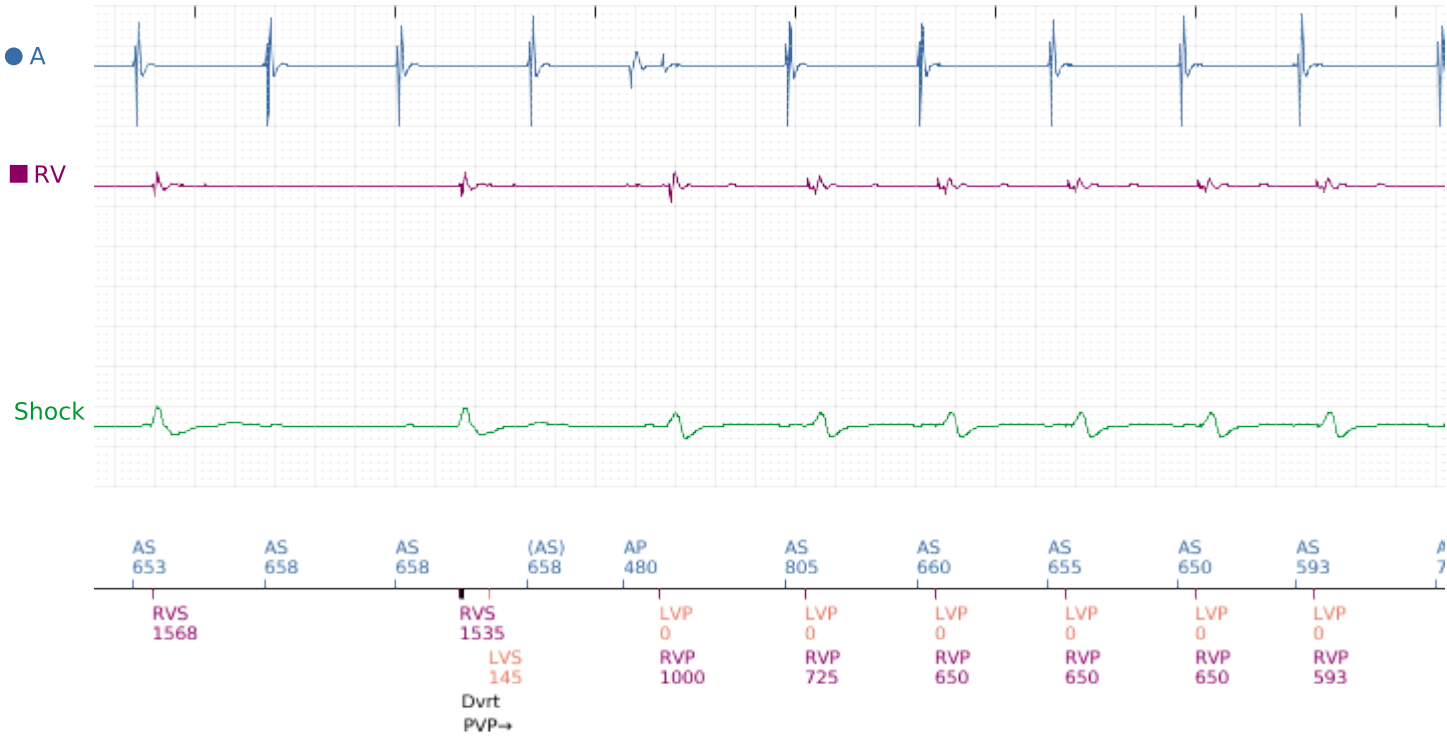

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

