



Date of Birth:
 Device: **RESONATE CRT-D G424/490880**
 Clinic:
 Search Tags:
 Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **15 Jun 2021 03:22 CEST**
 Last Office Interrogation: **19 May 2021**
 Implant Date:

V-42: 20 Apr 2021 00:54, VF, A Rate: 64 min⁻¹, V Rate: 321 min⁻¹

Detail

VF Event Onset

Avg A Rate 64 min⁻¹
 Avg V Rate 321 min⁻¹
 Detection Rhythm ID
 Template 13 Apr 2021 18:29
 RhythmMatch™ Threshold 94 %

At V-Detect

Avg A Rate 65 min⁻¹
 Avg V Rate 297 min⁻¹
 Rate Zone VF
 Stability (19 ms, Off)
 V>A Rate (True, Off)
 AFib (False, Off)
 RhythmID Correlated False
 RhythmMatch™ Too Fast
 SRD Met (False, Off)
 ATP Timeout False

Attempt 1, 41 J V Shock

Elapsed Time 00:00:06
 Shock Information
 Charge Time 9.8 s
 Lead Impedance 76 Ω
 Lead Polarity Initial


Event Ended


00:00:47

EGM displayed at 25mm per second





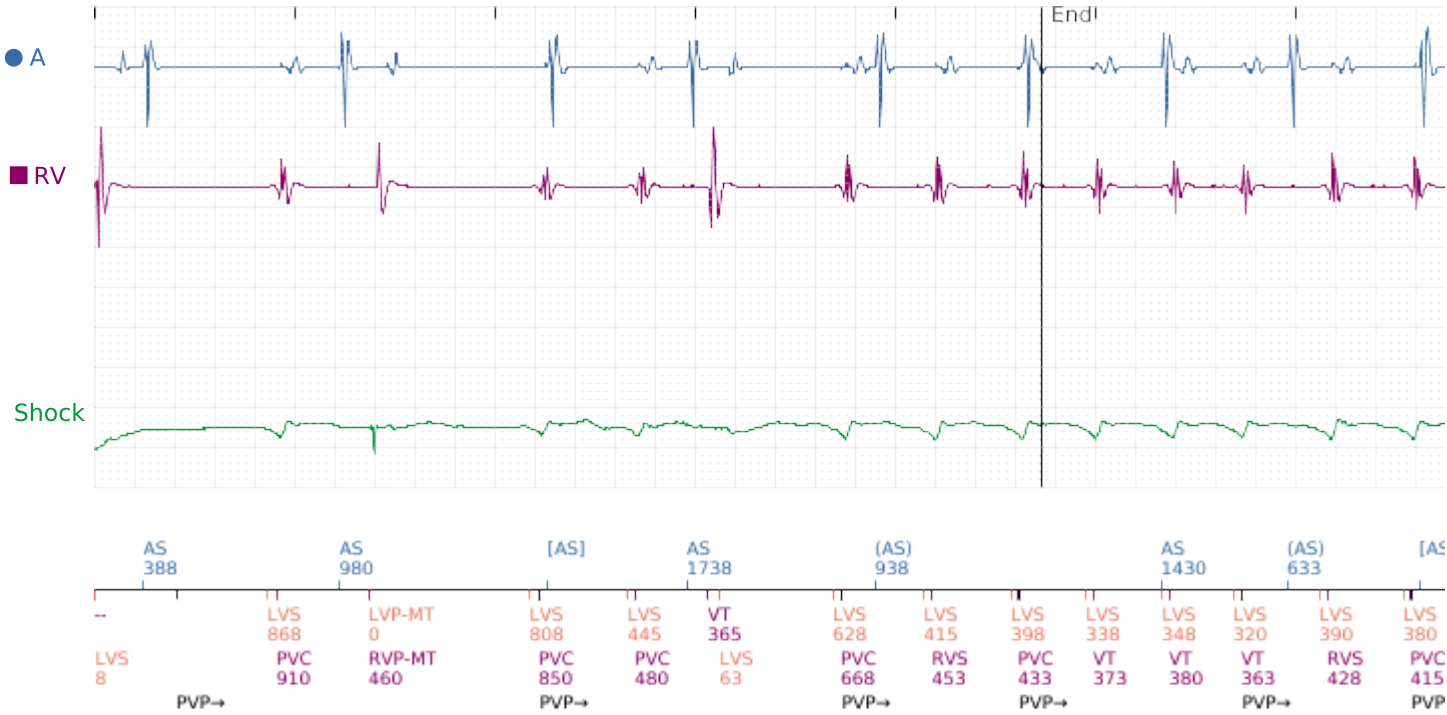

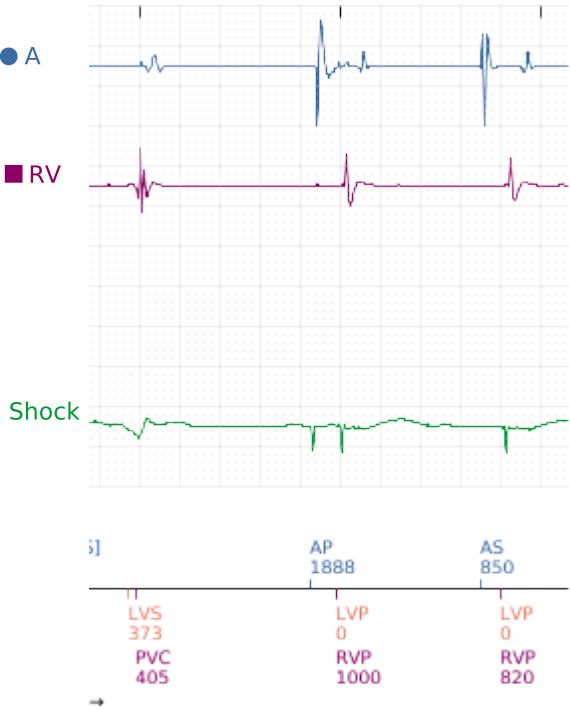

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

