



Date of Birth:
Device: **INCEPTA ICD F161**
Clinic:
Search Tags:
Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **28 Nov 2022 07:35 CET**
Last Office Interrogation: **08 Sep 2021**
Implant Date:
Patient Group:

V-35: 18 Oct 2019 07:28, VF, V Rate: 245 min⁻¹

Detail

VF Event Onset

Avg V Rate 245 min⁻¹
Detection Rate Only
Template 18 Oct 2019 05:40

At V-Detect

Avg V Rate 261 min⁻¹
Rate Zone VF
RhythmID Correlated False
RhythmMatch™ Too Fast
SRD Met (False, Off)
ATP Timeout False


Attempt 1, 14 J V Shock


Elapsed Time 00:00:03
Shock Information
Charge Time 2.7 s
Lead Impedance 33 Ω
Lead Polarity Initial


Event Ended

00:00:37

EGM displayed at 25mm per second

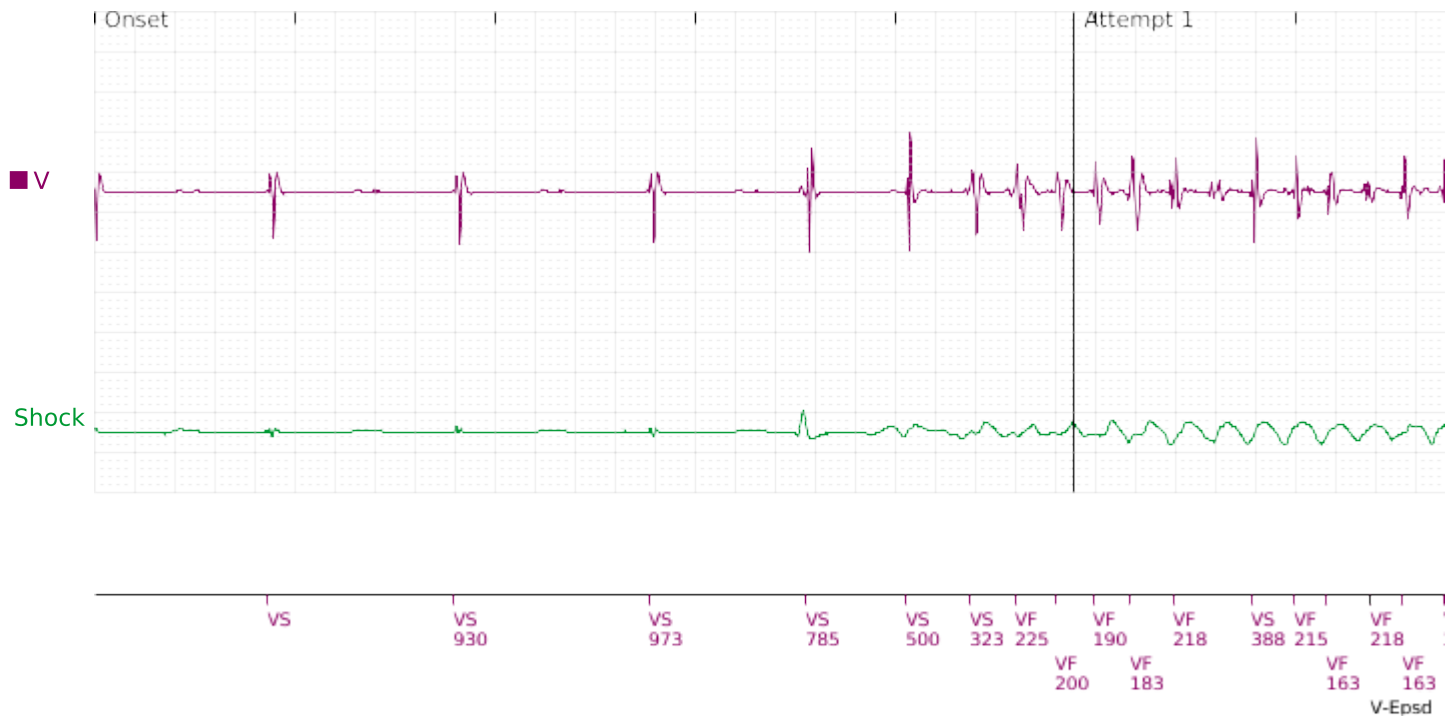

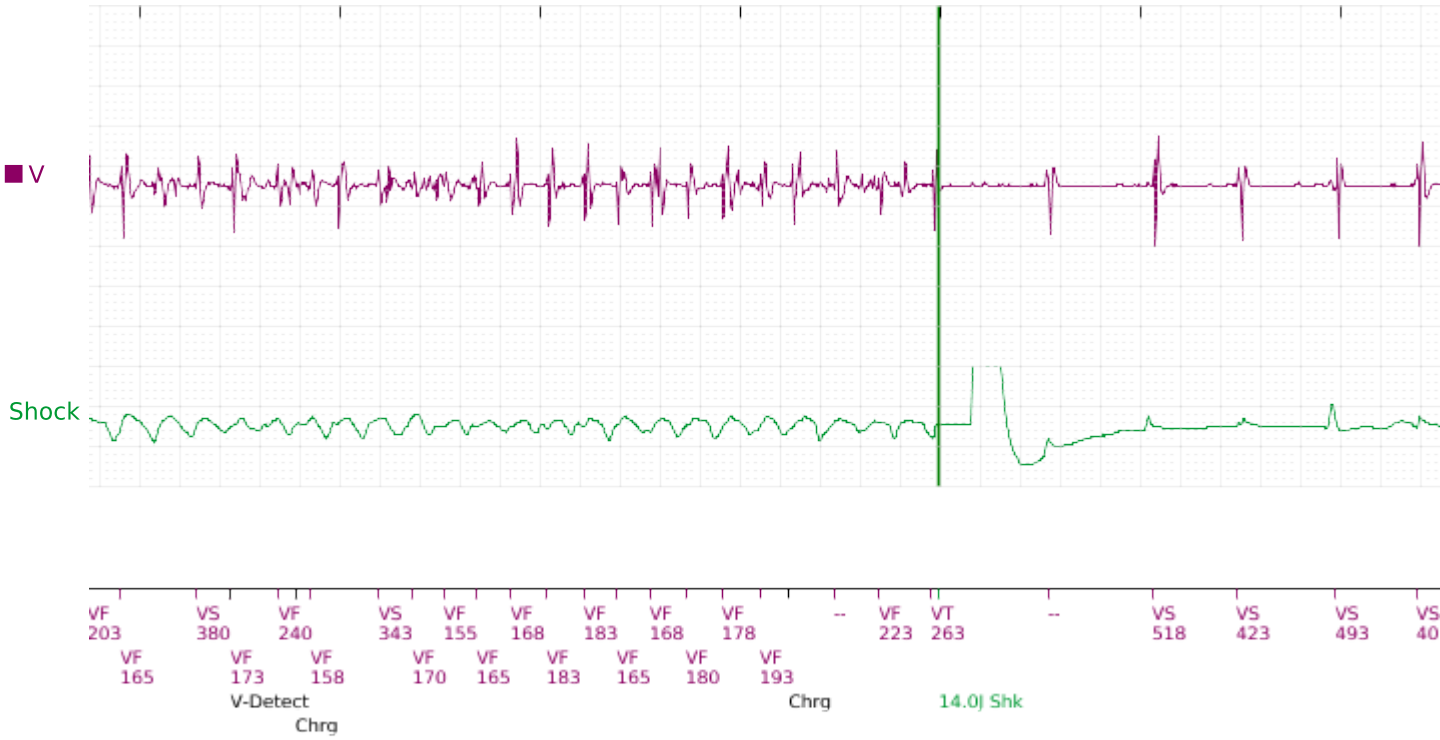

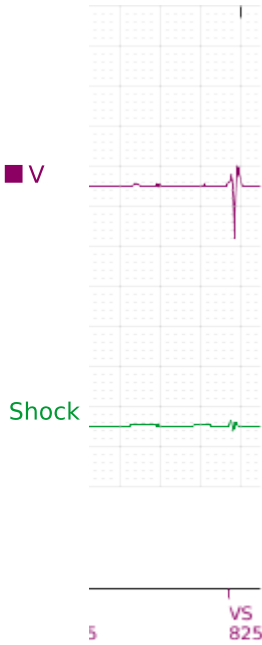

↑ > V Range

↓ < V Range

■ V Sense

□ V Pace

