

LATITUDE™ Patient Management - Event Detail Report		Report Created: 23 Jan 2023
	Date of Birth:	Latest Device Transmission: 12 Dec 2022 00:11 CET
	Device: RESONATE CRT-D	Last Office Interrogation: 01 Dec 2022
	Clinic:	Implant Date:
	Search Tags:	Patient Group:
	Tachy Mode: Monitor + Therapy	(Primary)

V-1: 10 Aug 2022 08:22, VF, A Rate: 111 min⁻¹, V Rate: 248 min⁻¹

Detail

VF Event Onset		
Avg A Rate	111 min ⁻¹	
Avg V Rate	248 min ⁻¹	
Detection	Rate Only	
Template	N/R	
At V-Detect		
Avg A Rate	79 min ⁻¹	
Avg V Rate	269 min ⁻¹	
Rate Zone	VF	
Stability	(21 ms, Off)	
V>A Rate	(True, Off)	
AFib	(False, Off)	
RhythmMatch™	N/R	
SRD Met	(False, Off)	
ATP Timeout	False	
Onset Intvl	(8 ms, Off)	
Onset %	(1 %, Off)	
Attempt 1, 41 J V Shock		
Elapsed Time		00:00:04
Shock Information		
Charge Time		9.4 s
Lead Impedance		77 Ω
Lead Polarity		Initial
At V-Detect		
Avg A Rate	131 min ⁻¹	
Avg V Rate	286 min ⁻¹	
Rate Zone	VF	
Stability	(59 ms, Off)	
V>A Rate	(True, Off)	
AFib	(False, Off)	
SRD Met	(False, Off)	
ATP Timeout	False	
Attempt 2, 41 J V Shock		
Elapsed Time		00:00:19
Shock Information		
Charge Time		7.2 s
Lead Impedance		76 Ω
Lead Polarity		Initial
At V-Detect		
Avg A Rate	99 min ⁻¹	
Avg V Rate	357 min ⁻¹	
Rate Zone	VF	
Stability	(64 ms, Off)	
V>A Rate	(True, Off)	
AFib	(False, Off)	
SRD Met	(False, Off)	
ATP Timeout	False	
Attempt 3, 41 J Max V Shock		
Elapsed Time		00:00:31
Shock Information		
Charge Time		7.1 s
Lead Impedance		76 Ω
Lead Polarity		Initial
At V-Detect		
Avg A Rate	111 min ⁻¹	
Avg V Rate	283 min ⁻¹	
Rate Zone	VF	
Stability	(10 ms, Off)	
V>A Rate	(True, Off)	
AFib	(False, Off)	
SRD Met	(False, Off)	
ATP Timeout	False	
Attempt 4, 41 J Max V Shock		
Elapsed Time		00:00:44
Shock Information		
Charge Time		7.1 s
Lead Impedance		76 Ω
Lead Polarity		Initial
At V-Detect		
Attempt 5, 41 J Max V Shock		

Clinician Signature

Clinician



Avg A Rate	88 min ⁻¹	Elapsed Time	00:00:56
Avg V Rate	274 min ⁻¹	Shock Information	
Rate Zone	VF	Charge Time	7.1 s
Stability	(9 ms, Off)	Lead Impedance	76 Ω
V>A Rate	(True, Off)	Lead Polarity	Initial
AFib	(False, Off)		
SRD Met	(False, Off)		
ATP Timeout	False		



Event Ended



00:01:35


EGM displayed at 25mm per second




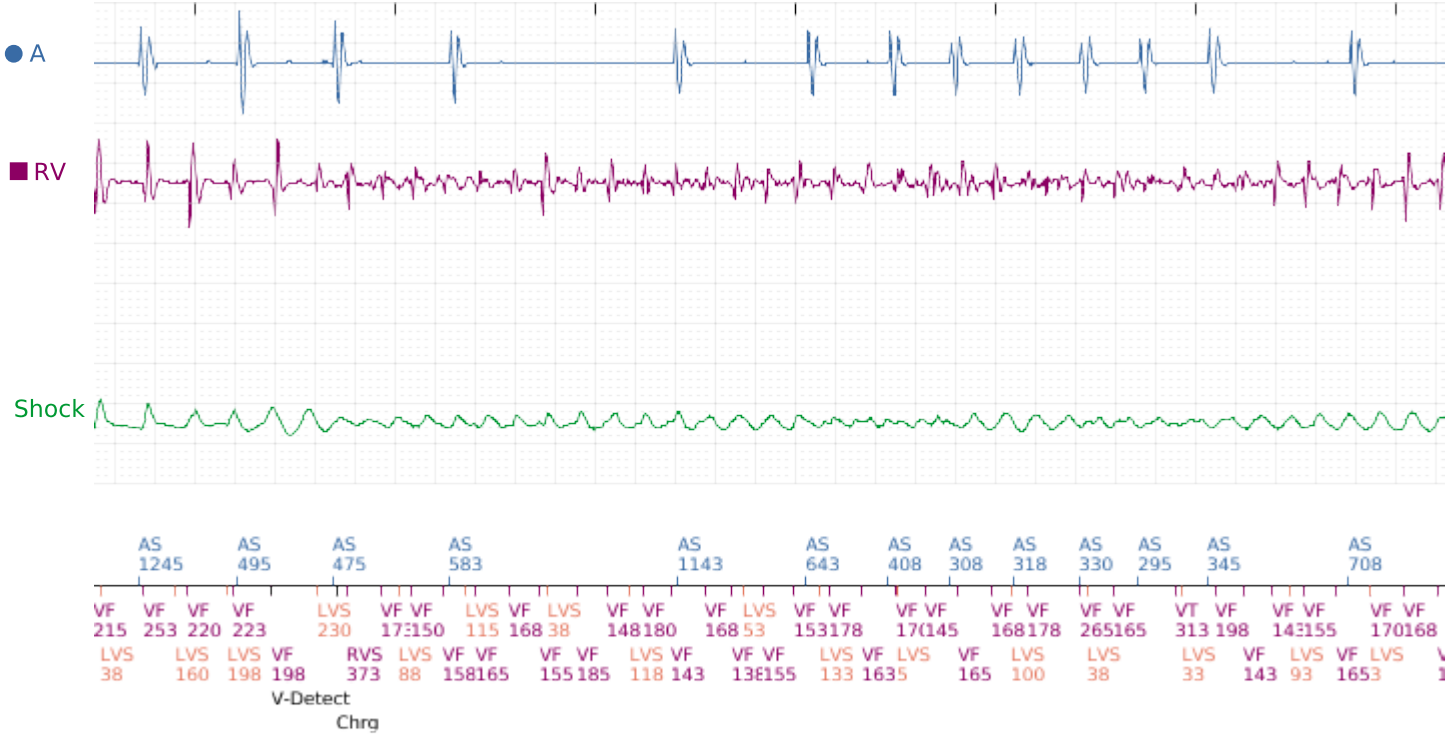
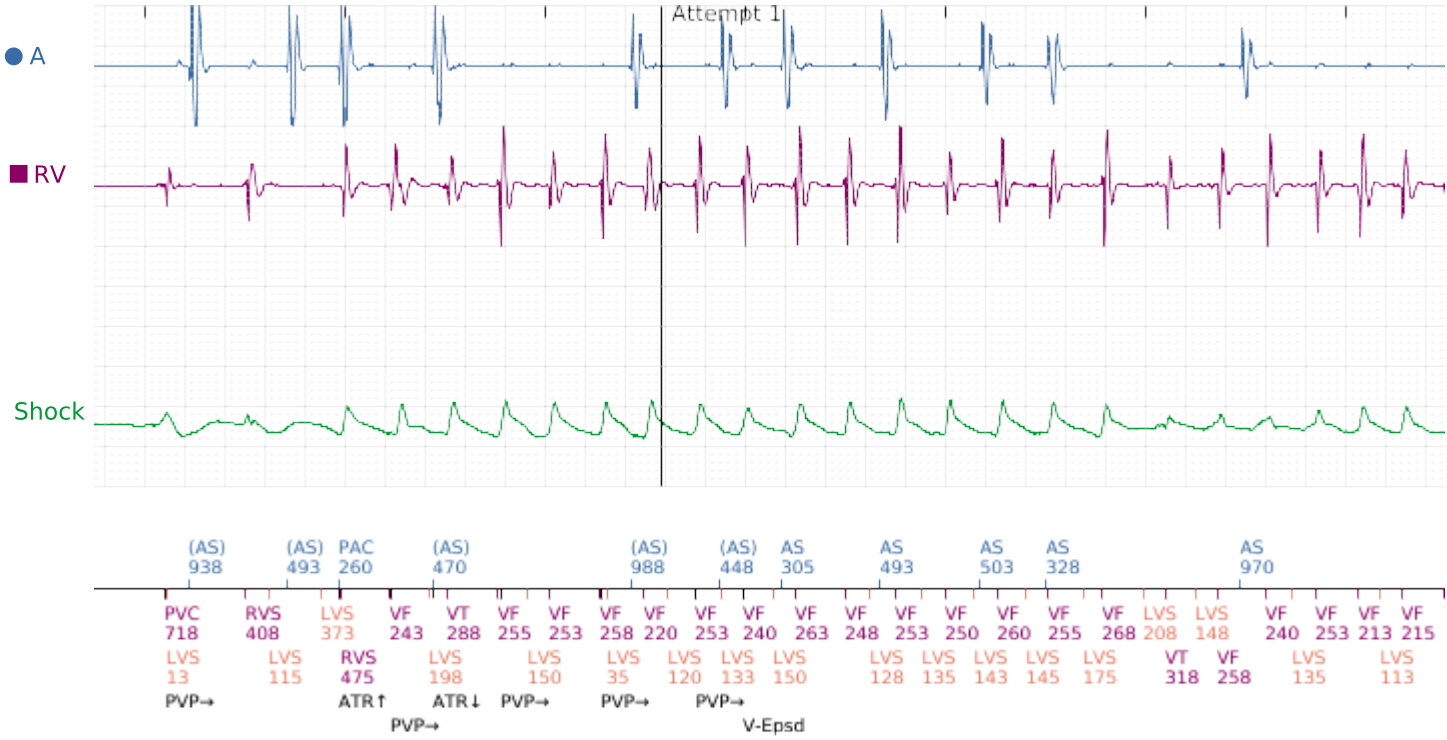


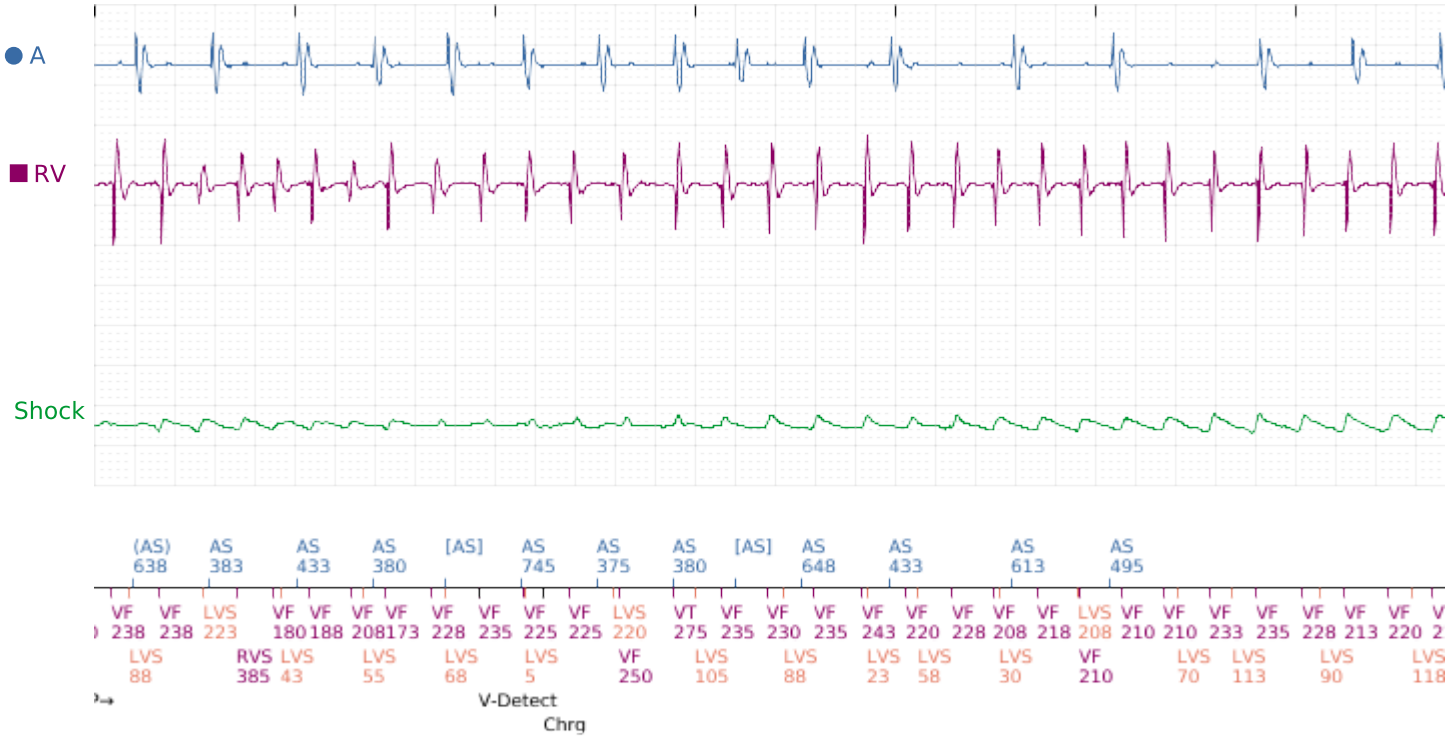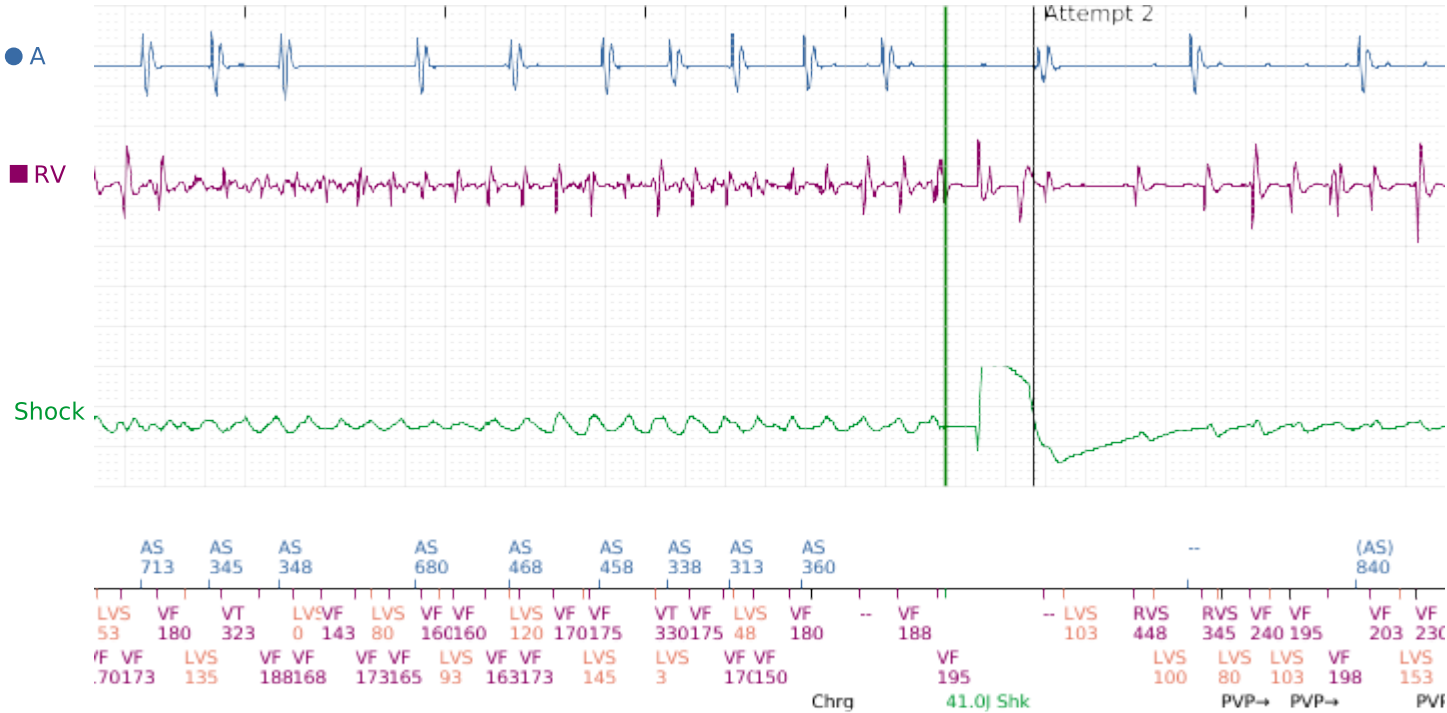

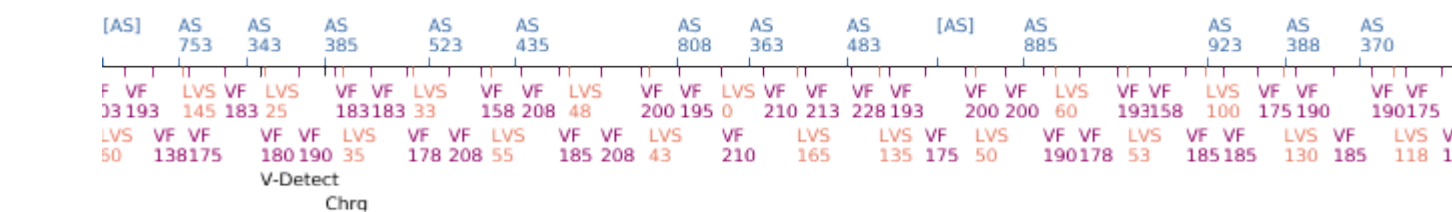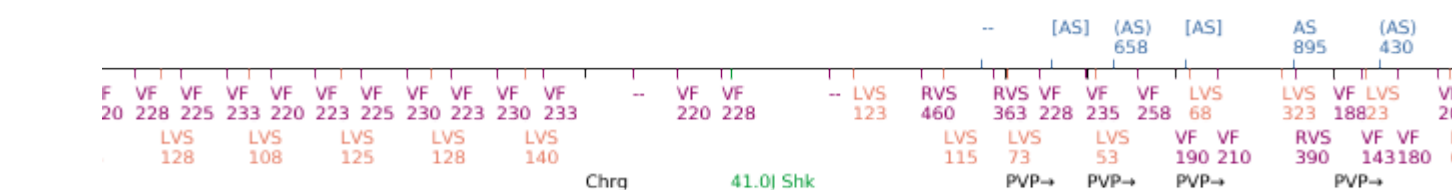

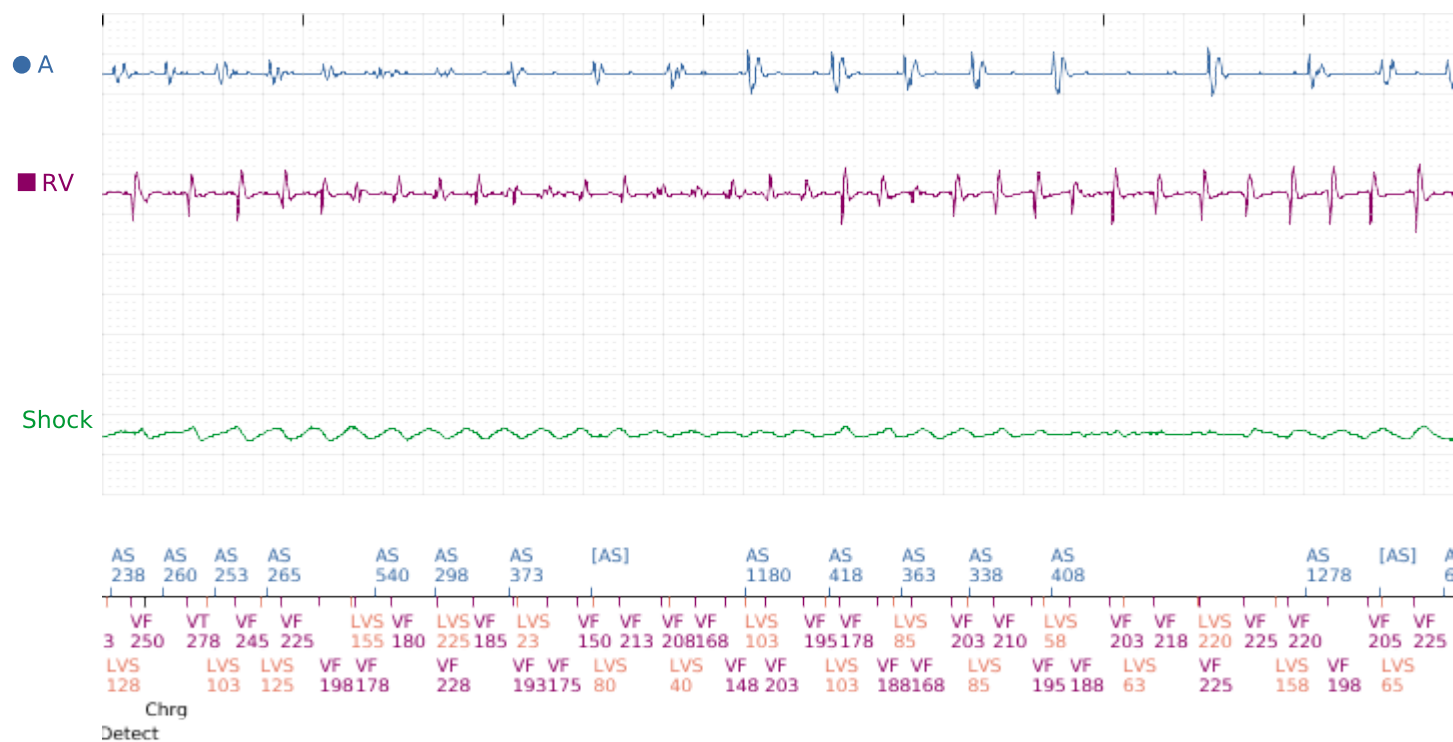

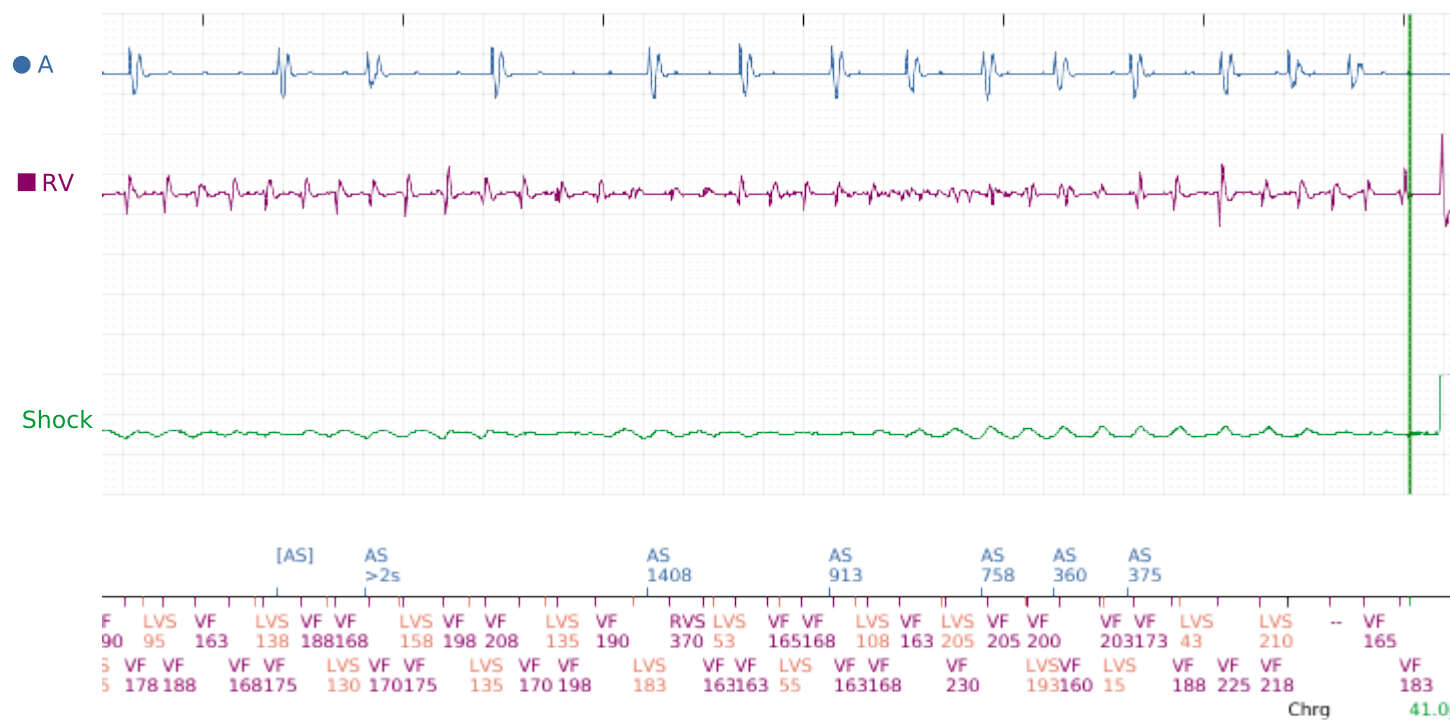

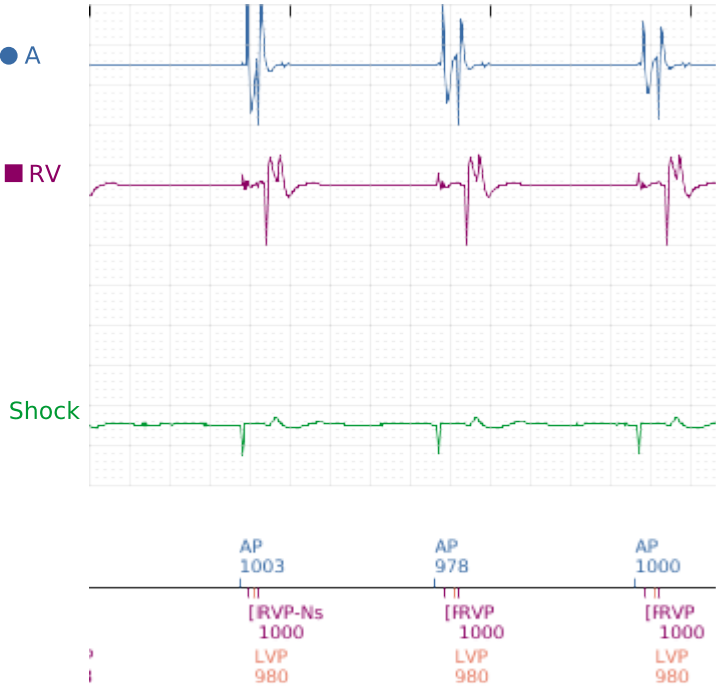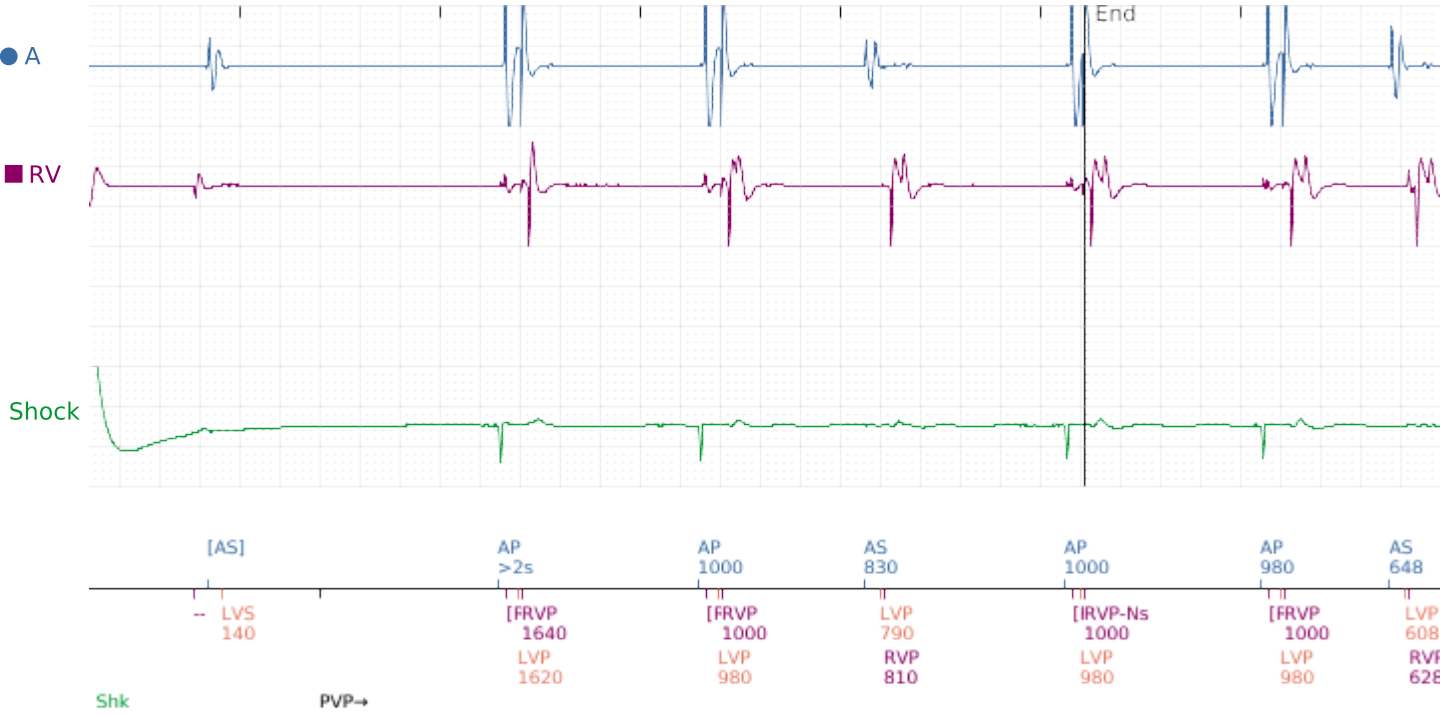

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

