



Date of Birth:
 Device: **AUTOGEN EL ICD D176**
 Clinic:
 Search Tags:
 Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **24 Jan 2023 00:50 CET**
 Last Office Interrogation: **01 Dec 2022**
 Implant Date:
 Patient Group:

V-106: 14 Mar 2019 03:22, VF, A Rate: 42 min⁻¹, V Rate: 240 min⁻¹

Detail

VF Event Onset

Avg A Rate 42 min⁻¹
 Avg V Rate 240 min⁻¹
 Detection Rhythm ID
 Template 13 Mar 2019 19:41
 RhythmMatch™ Threshold 94 %

At V-Detect

Avg A Rate 47 min⁻¹
 Avg V Rate 279 min⁻¹
 Rate Zone VF
 Stability (69 ms, Off)
 V>A Rate (True, Off)
 AFib (False, Off)
 RhythmID Correlated False
 RhythmMatch™ 30 %
 SRD Met (False, Off)
 ATP Timeout False


Attempt 1, 41 J V Shock



Elapsed Time 00:00:03
 VF ATP delivered prior to shock
 Shock Information
 Charge Time 9.7 s
 Lead Impedance 60 Ω
 Lead Polarity Initial



Event Ended

00:00:48

EGM displayed at 25mm per second

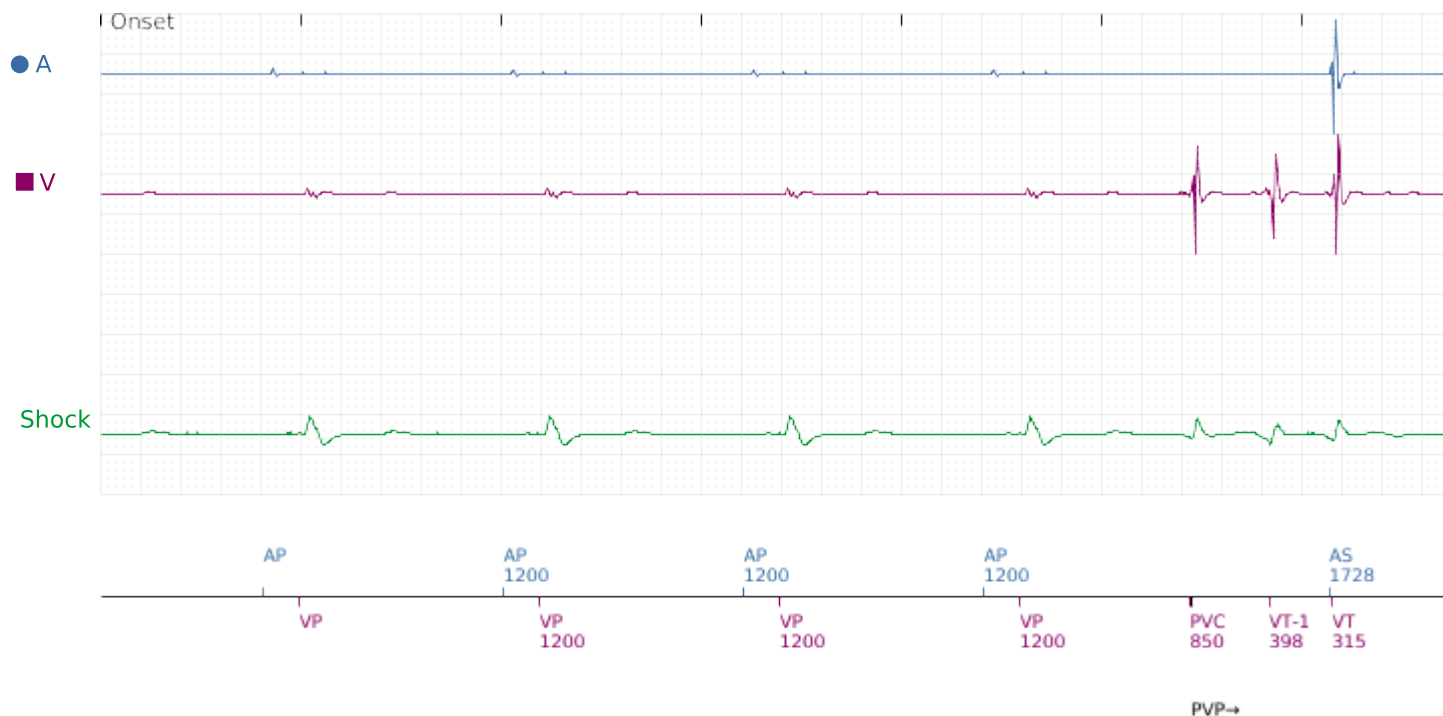

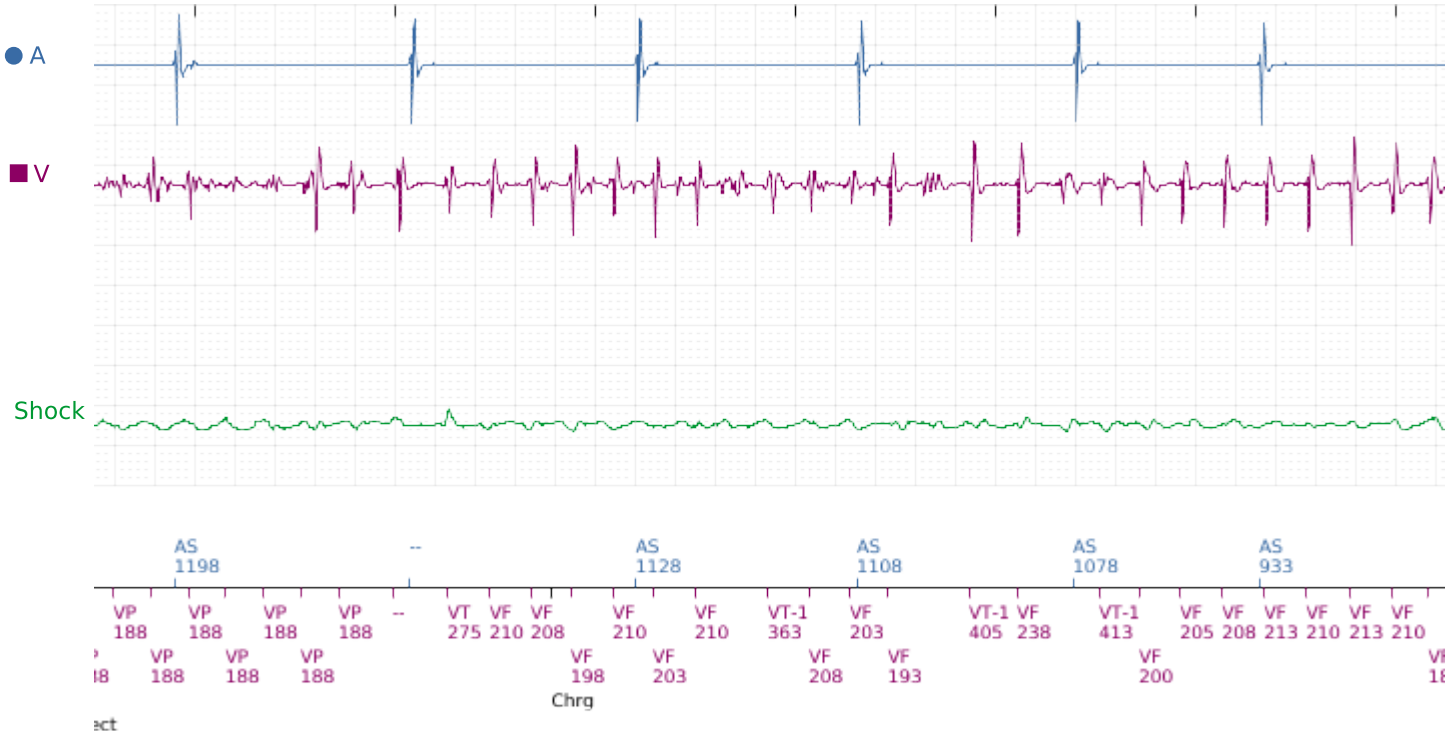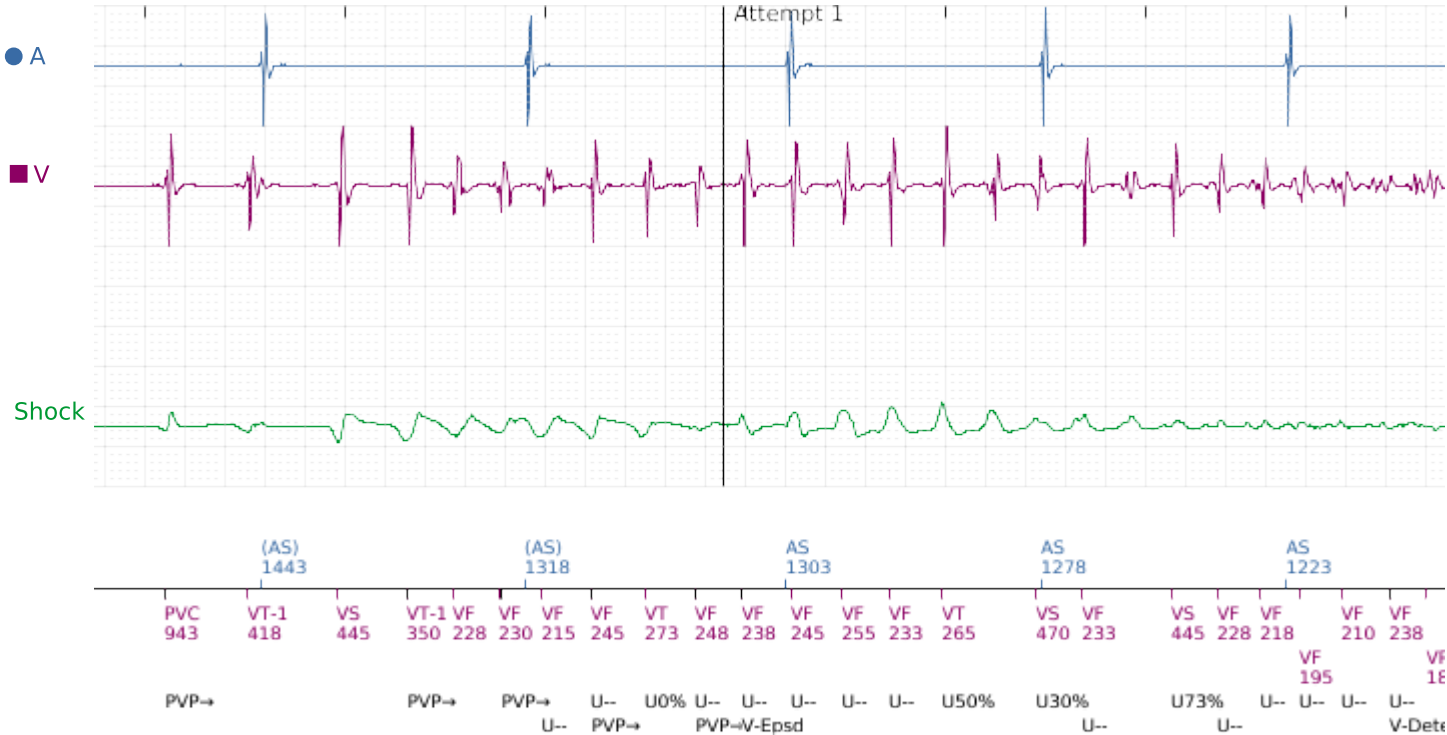

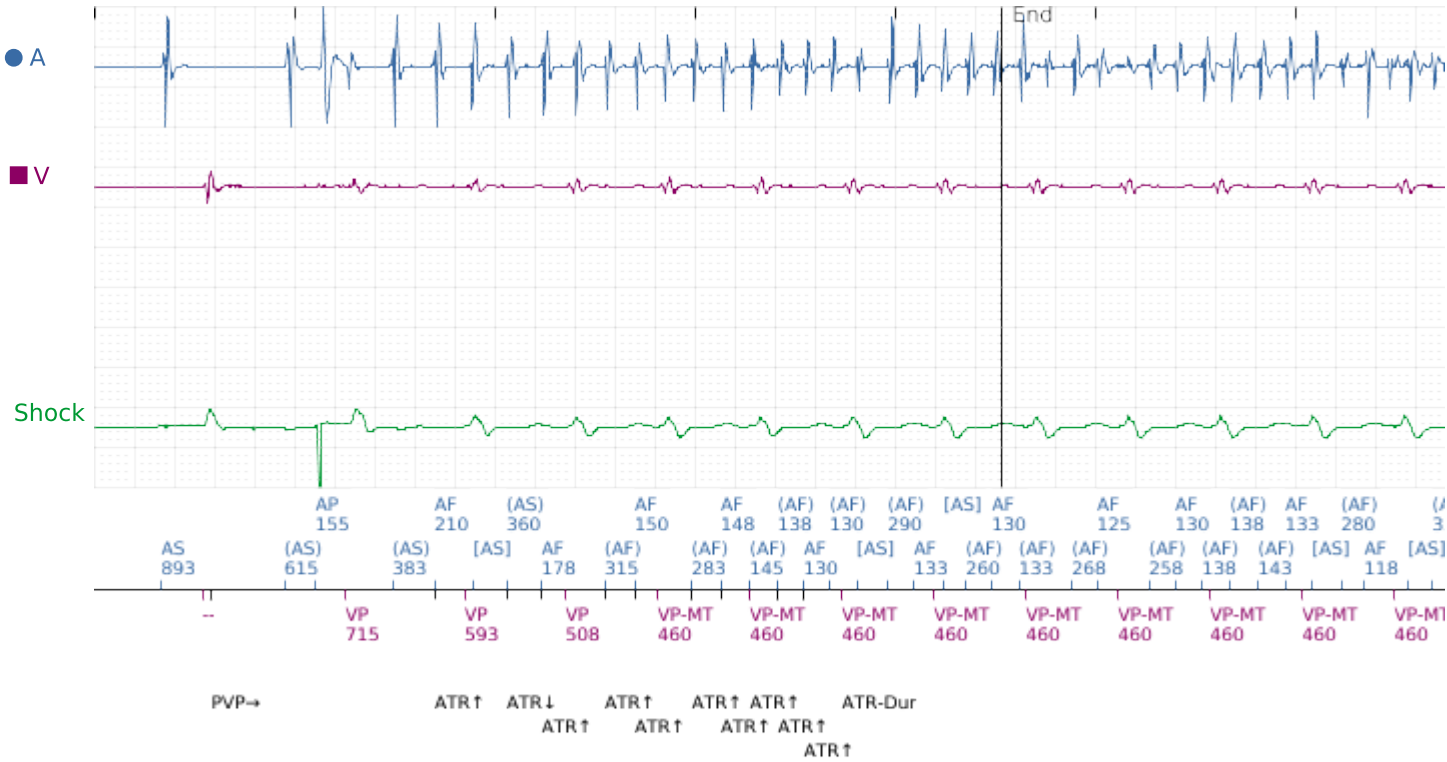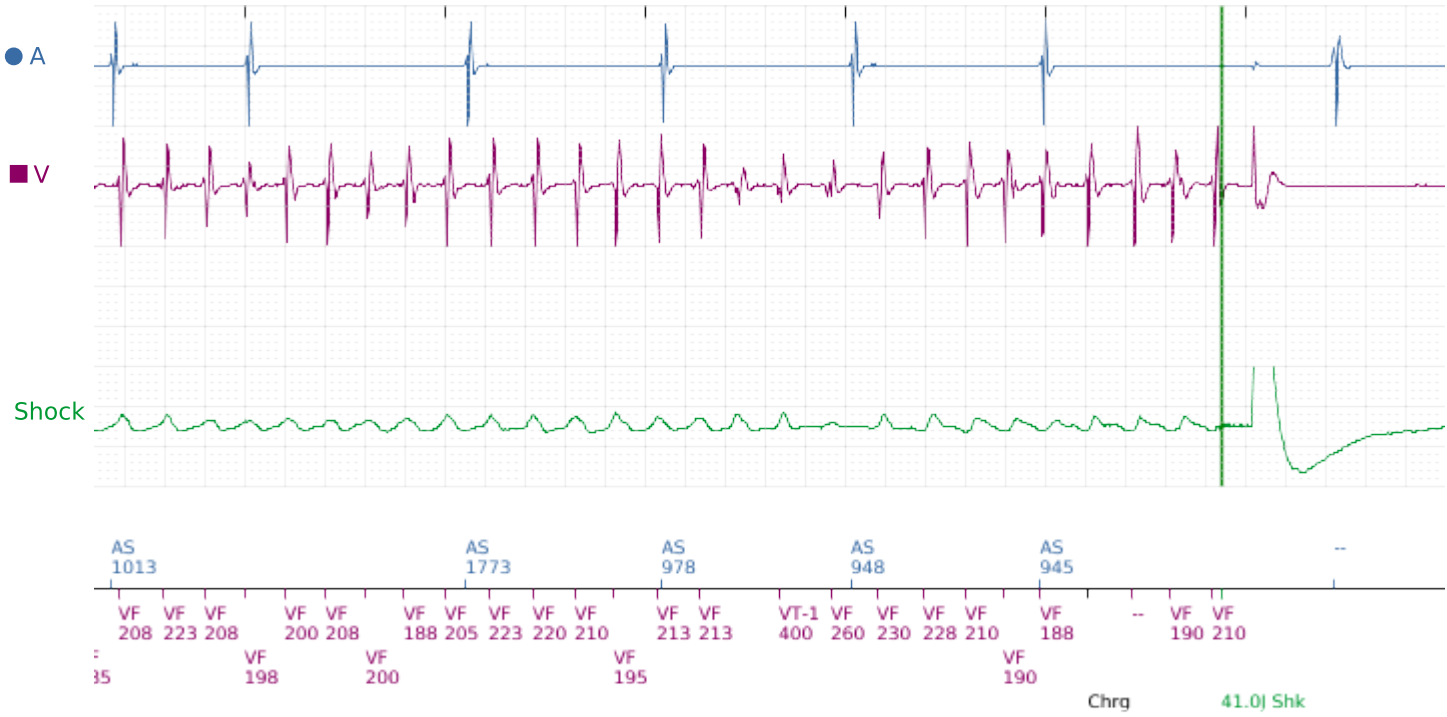



↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	○ A Pace

