



Date of Birth:
 Device: **INCEPTA CRT-D P162**
 Clinic:
 Search Tags:
 Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **16 Oct 2017 03:01 CEST**
 Last Office Interrogation: **28 Sep 2017**
 Implant Date:
 Patient Group:

V-3205: 31 Oct 2014 19:11, VF, A Rate: 30 min⁻¹, V Rate: 224 min⁻¹

Detail

VF Event Onset

Avg A Rate 30 min⁻¹
 Avg V Rate 224 min⁻¹
 Detection Rate Only
 Template N/R

At V-Detect

Avg A Rate 30 min⁻¹
 Avg V Rate 226 min⁻¹
 Rate Zone VF
 Stability (8 ms, Off)
 V>A Rate (True, Off)
 AFib (False, Off)
 RhythmMatch™ N/R
 SRD Met (False, Off)
 ATP Timeout False
 Onset Intvl (68 ms, Off)
 Onset % (11 %, Off)


Attempt 1, 31 J V Shock


Elapsed Time 00:00:03
 VF ATP delivered prior to shock
 Shock Information
 Charge Time 6.0 s
 Lead Impedance 74 Ω
 Lead Polarity Initial


Event Ended

00:00:45

EGM displayed at 25mm per second

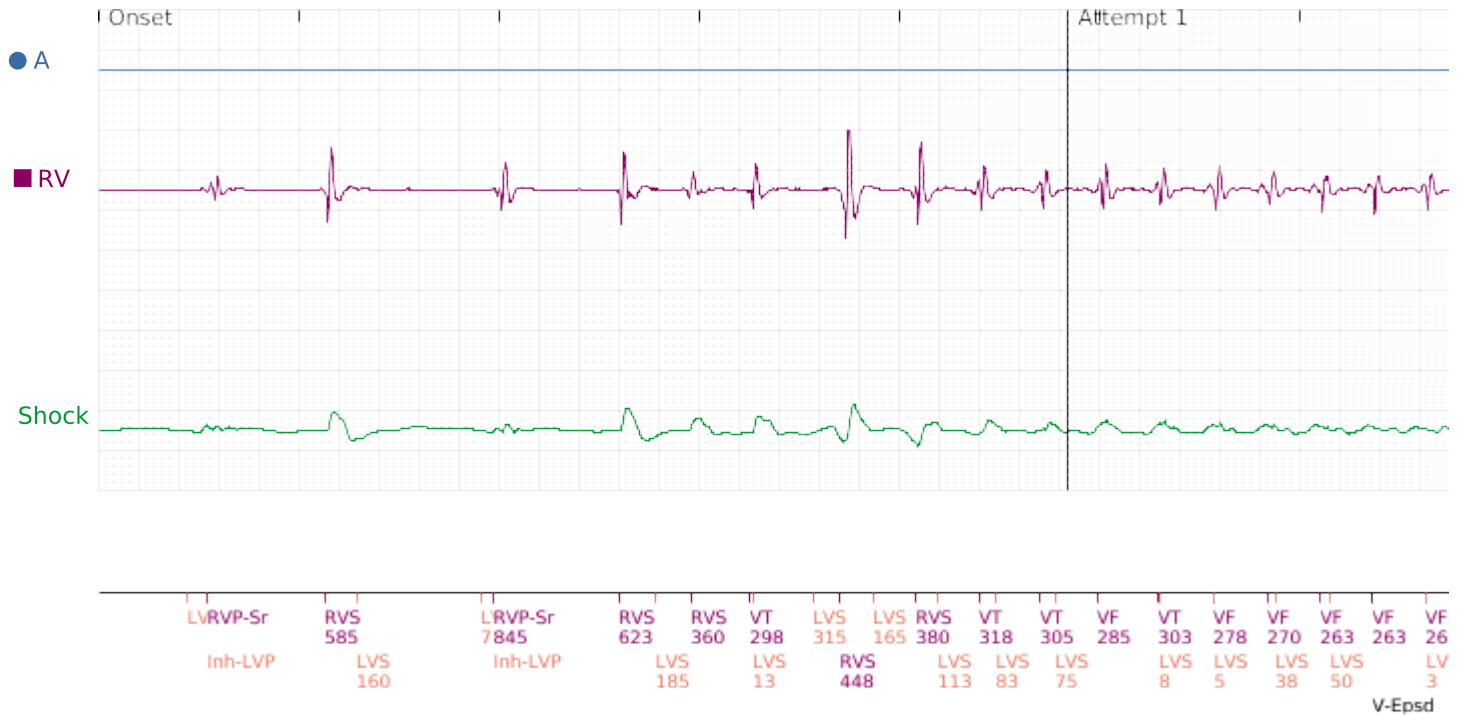

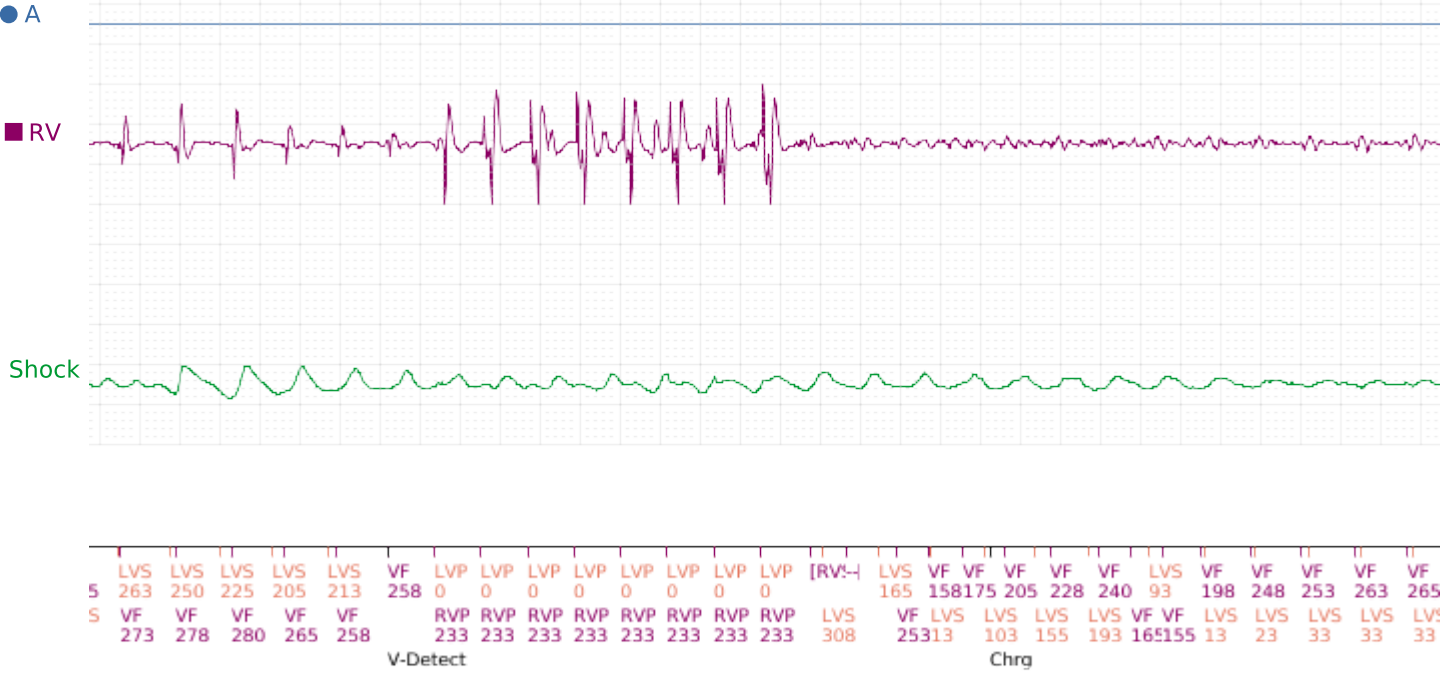

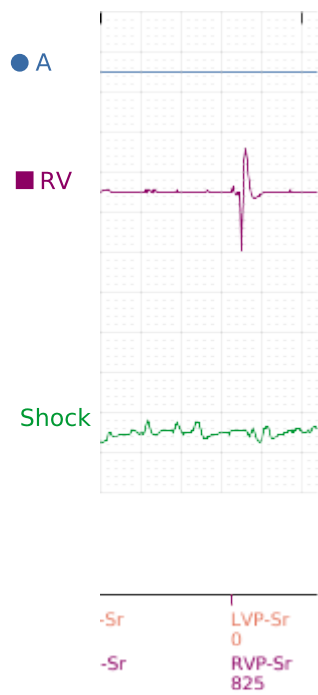

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

