



Date of Birth:
 Device: **AUTOGEN EL ICD D176**
 Clinic:
 Search Tags:
 Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **12 Dec 2022 03:41 CET**
 Last Office Interrogation: **16 Dec 2021**
 Implant Date:
 Patient Group:

V-29: 23 Jun 2018 12:58, VF, A Rate: 98 min⁻¹, V Rate: 343 min⁻¹

Detail

VF Event Onset

Avg A Rate 98 min⁻¹
 Avg V Rate 343 min⁻¹
 Detection Rhythm ID
 Template 23 Jun 2018 11:24
 RhythmMatch™ Threshold 94 %

At V-Detect

Avg A Rate 127 min⁻¹
 Avg V Rate 225 min⁻¹
 Rate Zone VF
 Stability (81 ms, Off)
 V>A Rate (True, Off)
 AFib (False, Off)
 RhythmID Correlated False
 RhythmMatch™ Too Fast
 SRD Met (False, Off)
 ATP Timeout False

Attempt 1, 41 J V Shock



Elapsed Time 00:00:03
 VF ATP delivered prior to shock
 Shock Information
 Charge Time 10.1 s
 Lead Impedance 66 Ω
 Lead Polarity Initial

Event Ended


00:00:48

EGM displayed at 25mm per second



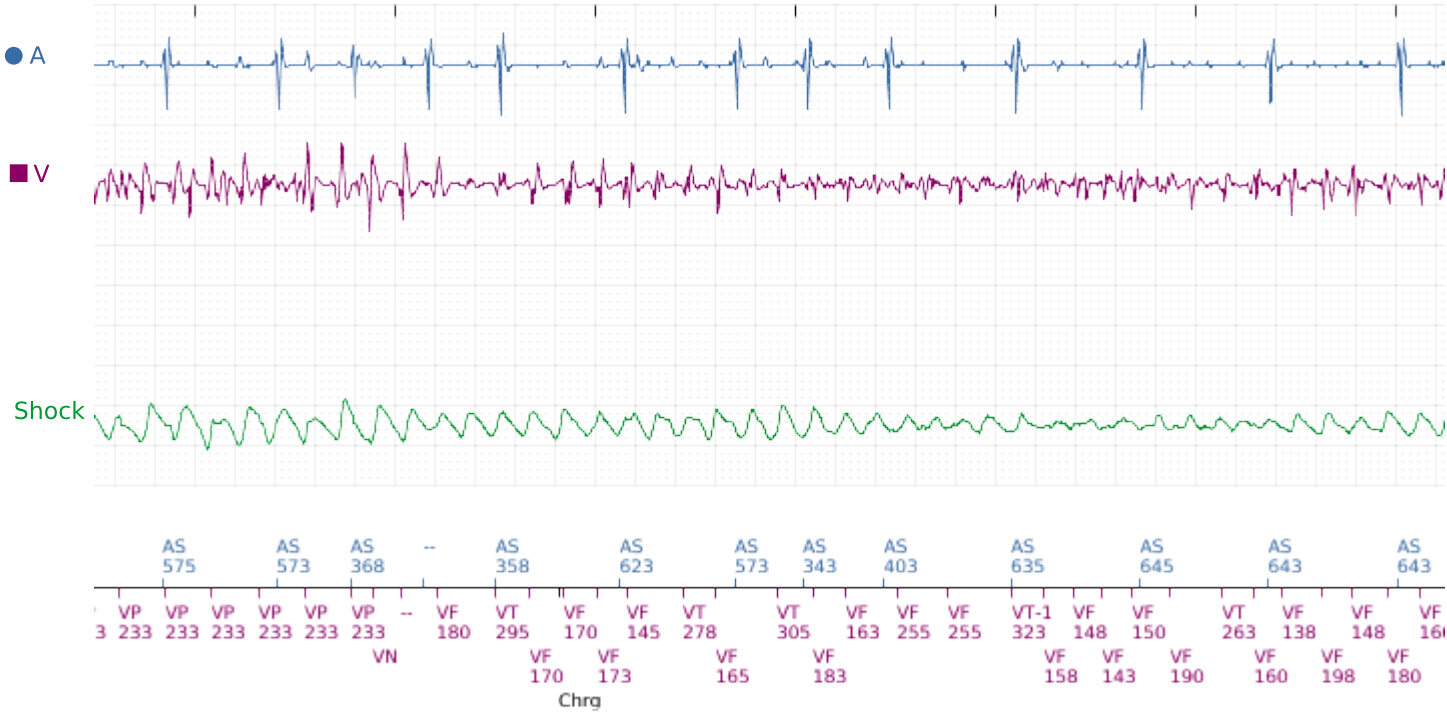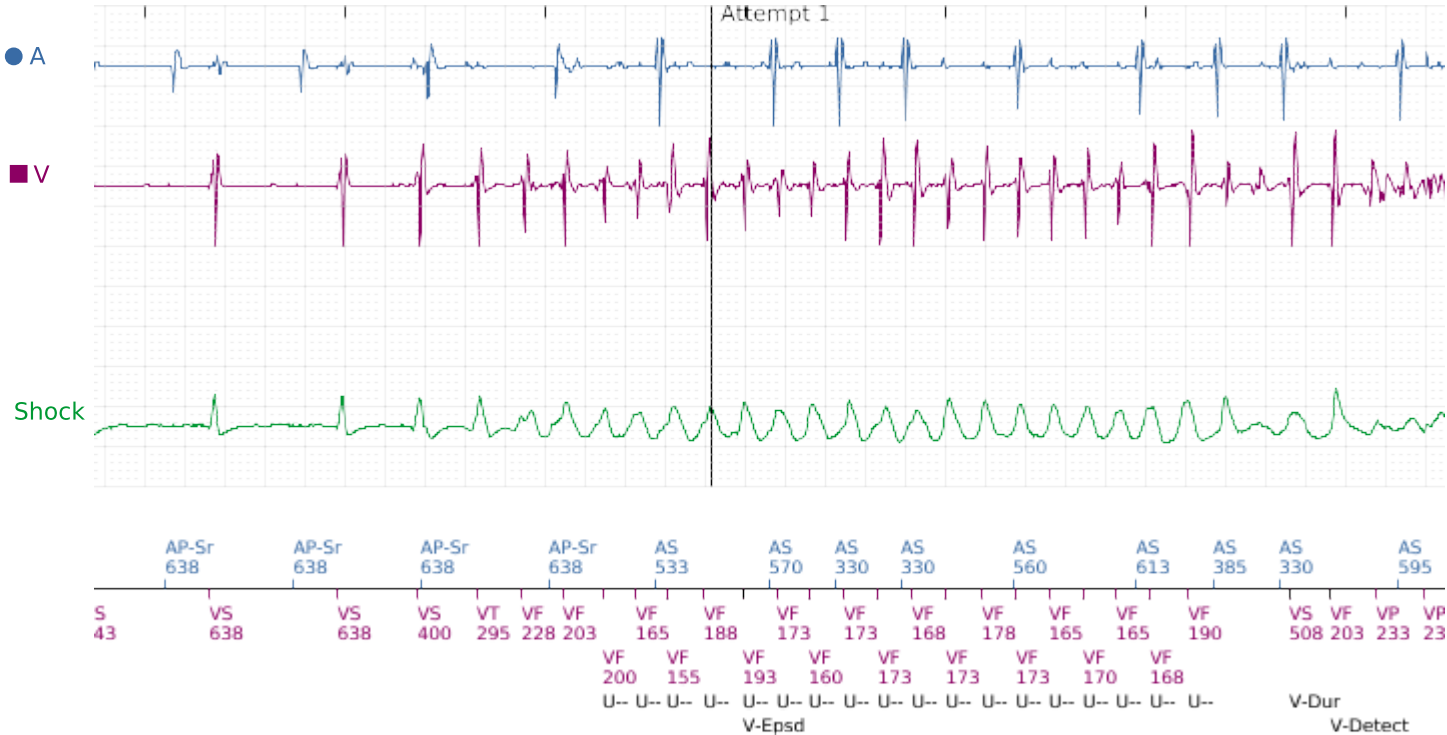



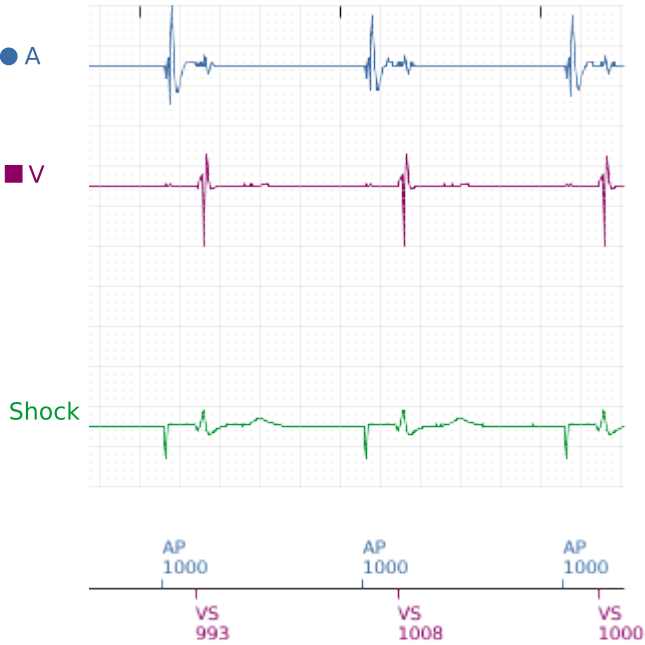

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

