



Date of Birth:  
Device: **MOMENTUM X4 CRT-D**

Clinic:  
Search Tags:  
Tachy Mode: **Monitor + Therapy**

Latest Device Transmission: **25 Apr 2022 00:21 CEST**

Last Office Interrogation: **18 Mar 2022**

Implant Date:  
Patient Group:

V-56: 15 Mar 2022 20:03, VT, A Rate: 78 min<sup>-1</sup>, V Rate: 180 min<sup>-1</sup>

## Detail

### VT Event Onset

|                        |                       |
|------------------------|-----------------------|
| Avg A Rate             | 78 min <sup>-1</sup>  |
| Avg V Rate             | 180 min <sup>-1</sup> |
| Detection              | Rhythm ID             |
| Template               | N/R                   |
| RhythmMatch™ Threshold | 94 %                  |

### At V-Detect

|                     |                       |
|---------------------|-----------------------|
| Avg A Rate          | 85 min <sup>-1</sup>  |
| Avg V Rate          | 173 min <sup>-1</sup> |
| Rate Zone           | VT                    |
| Stability           | 4 ms                  |
| V>A Rate            | True                  |
| AFib                | False                 |
| RhythmID Correlated | False                 |
| RhythmMatch™        | N/R                   |
| SRD Met             | (False, Off)          |
| ATP Timeout         | False                 |

### Attempt 1, Burst V ATP

|                  |          |
|------------------|----------|
| Elapsed Time     | 00:00:13 |
| ATP Information  |          |
| Number of Bursts | 1        |


Event Ended


00:00:27

### EGM displayed at 25mm per second





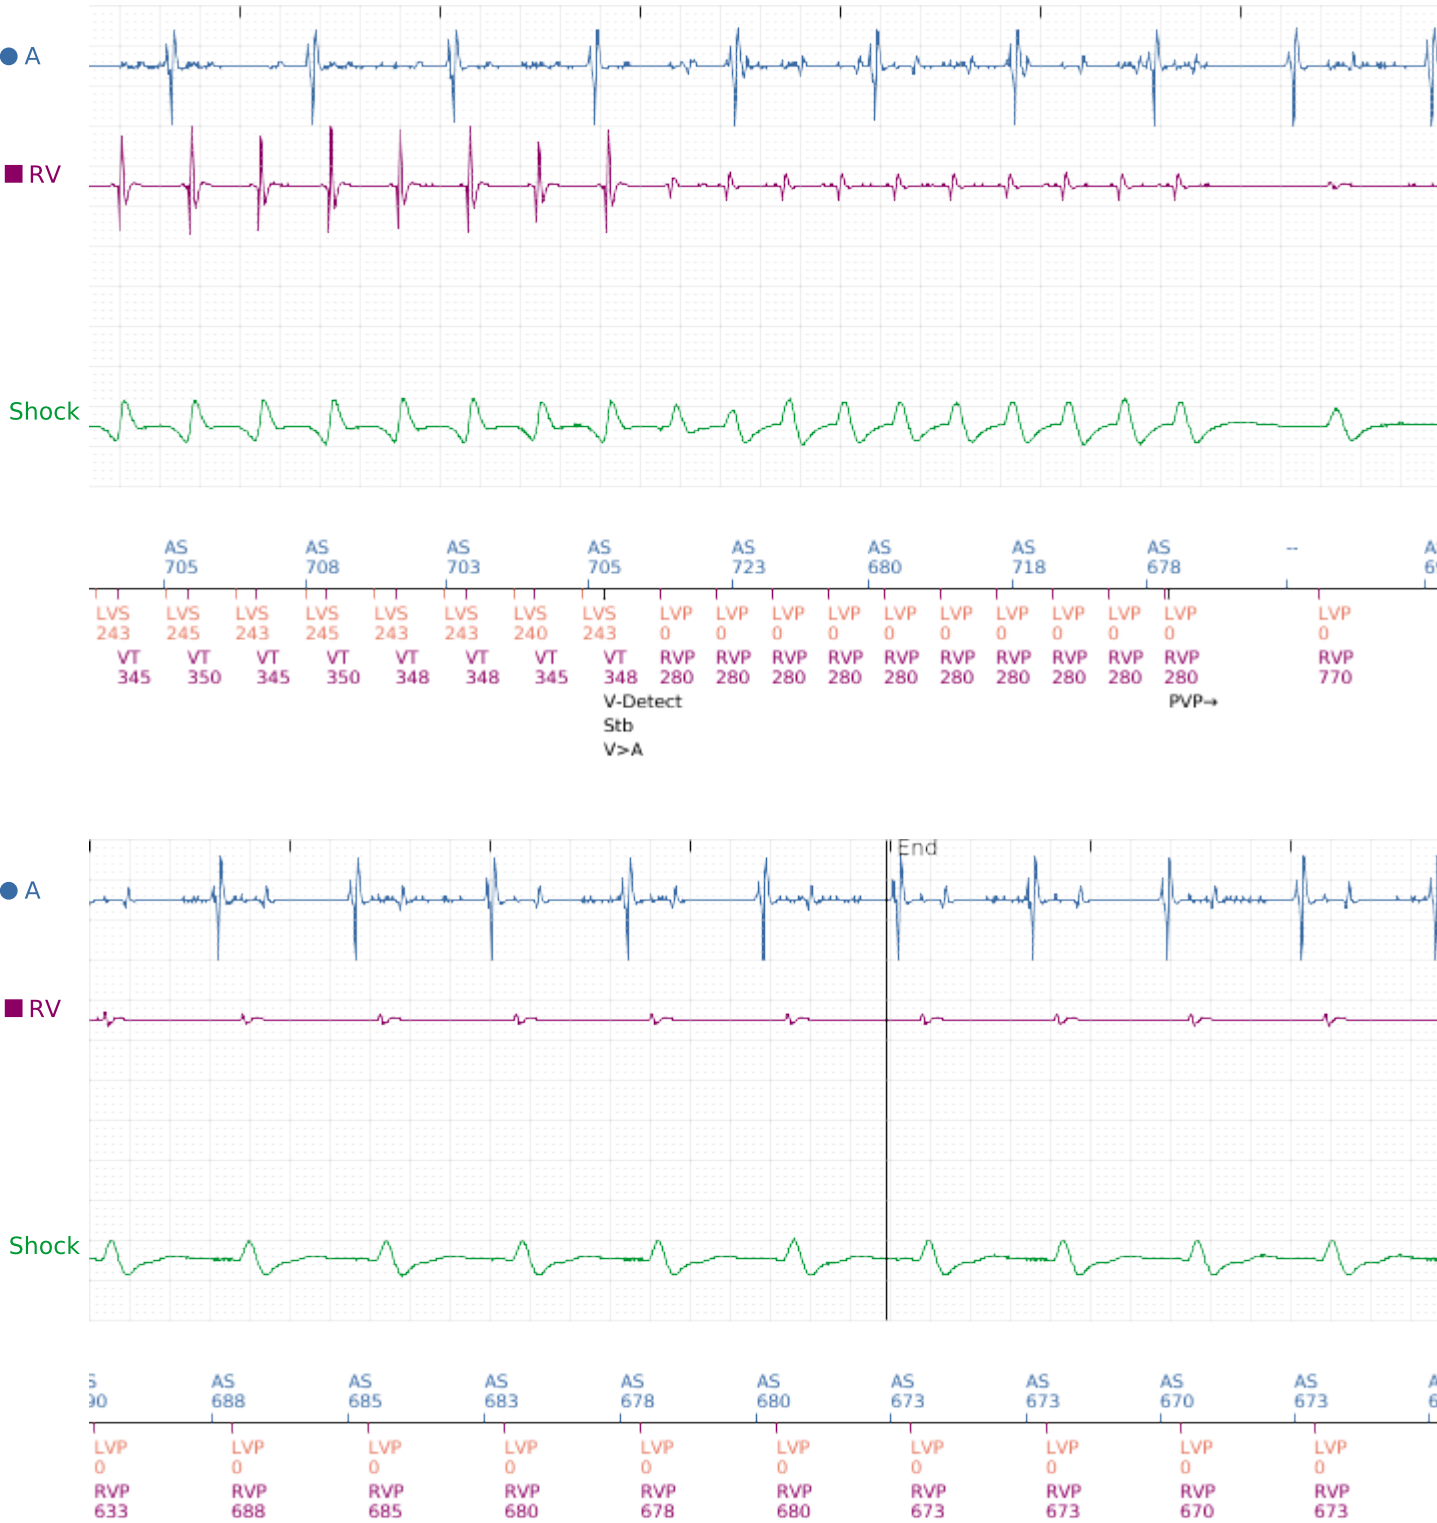

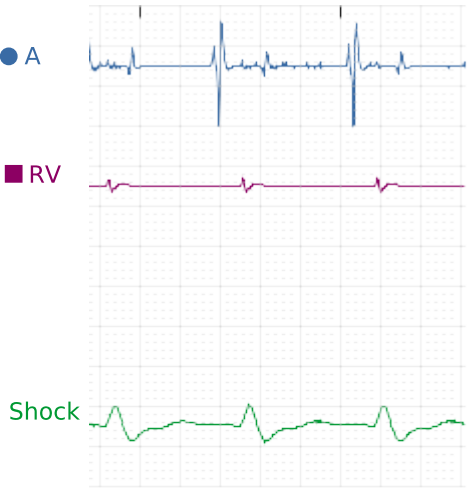

|            |            |            |
|------------|------------|------------|
| S<br>70    | AS<br>670  | AS<br>670  |
| LVP<br>0   | LVP<br>0   | LVP<br>0   |
| RVP<br>670 | RVP<br>670 | RVP<br>670 |

|             |             |           |          |
|-------------|-------------|-----------|----------|
| ↑ > V Range | ↓ < V Range | ■ V Sense | □ V Pace |
| ↑ > A Range | ↓ < A Range | • A Sense | ◦ A Pace |

