

LATITUDE™ Patient Management - Event Detail Report		Report Created: 23 Jan 2023
	Date of Birth:	Latest Device Transmission: 31 Oct 2022 00:11 CET
	Device: RESONATE X4 CRT-D	Last Office Interrogation: 03 Jun 2021
	Clinic:	Implant Date:
	Search Tags:	nt Group:
	Tachy Mode: Monitor + Therapy	


V-40: 27 May 2021 14:40, VT, A Rate: 98 min⁻¹, V Rate: 217 min⁻¹


Detail


VT Event Onset			
Avg A Rate	98 min ⁻¹		
Avg V Rate	217 min ⁻¹		
Detection	Rhythm ID		
Template	04 Apr 2021 12:27		
RhythmMatch™ Threshold	94 %		
At V-Detect			
Avg A Rate	109 min ⁻¹	Attempt 1, Burst V ATP	
Avg V Rate	205 min ⁻¹	Elapsed Time	00:00:30
Rate Zone	VT	ATP Information	
Stability	3 ms	Number of Bursts	4
V>A Rate	True		
AFib	False		
RhythmID Correlated	False		
RhythmMatch™	69 %		
SRD Met	(False, Off)		
ATP Timeout	False		
At V-Detect			
Avg A Rate	112 min ⁻¹	Attempt 2, Ramp V ATP	
Avg V Rate	202 min ⁻¹	Elapsed Time	00:00:56
Rate Zone	VT	ATP Information	
ATP Timeout	False	Number of Bursts	4
At V-Detect			
Avg A Rate	109 min ⁻¹	Attempt 3, 11 J V Shock	
Avg V Rate	233 min ⁻¹	Elapsed Time	00:01:28
Rate Zone	VT	Shock Information	
ATP Timeout	False	Charge Time	2.0 s
		Lead Impedance	60 Ω
		Lead Polarity	Initial
Event Ended			00:02:01

EGM displayed at 25mm per second

Clinician Signature

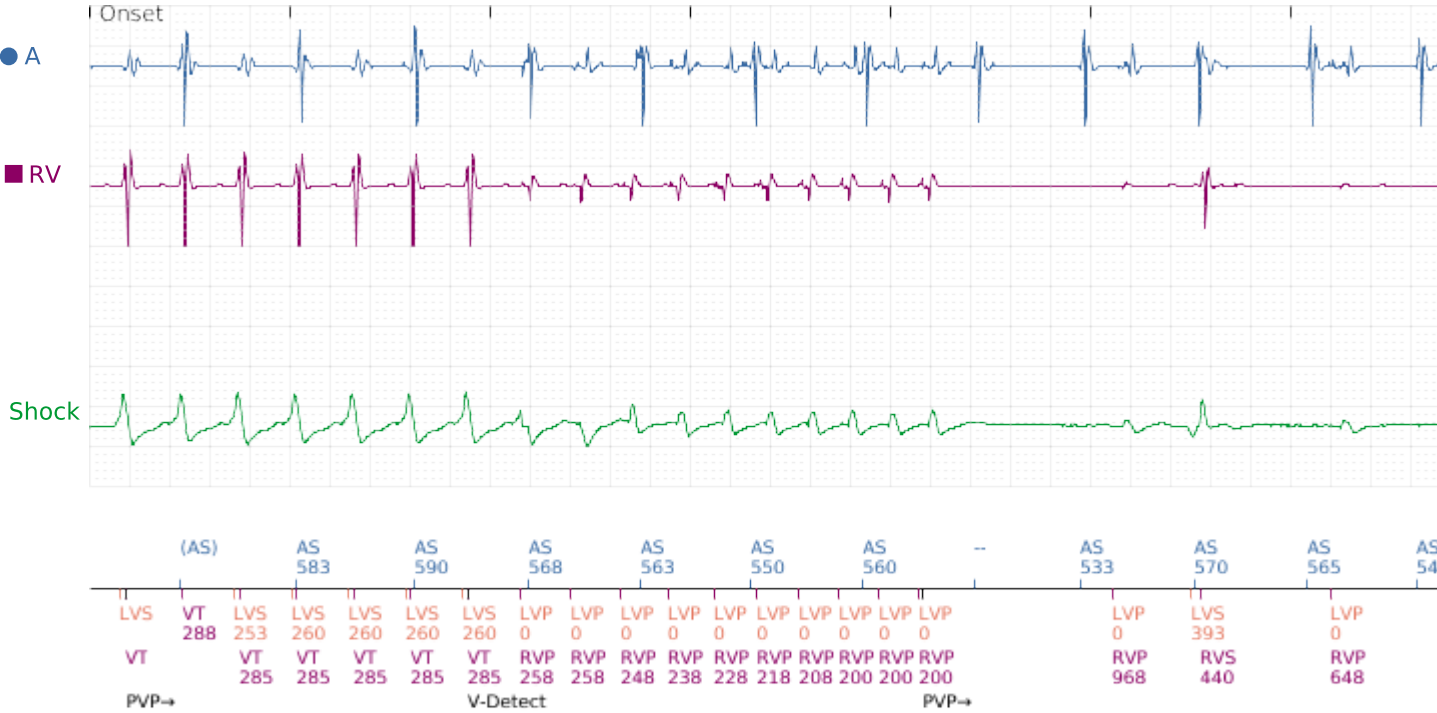



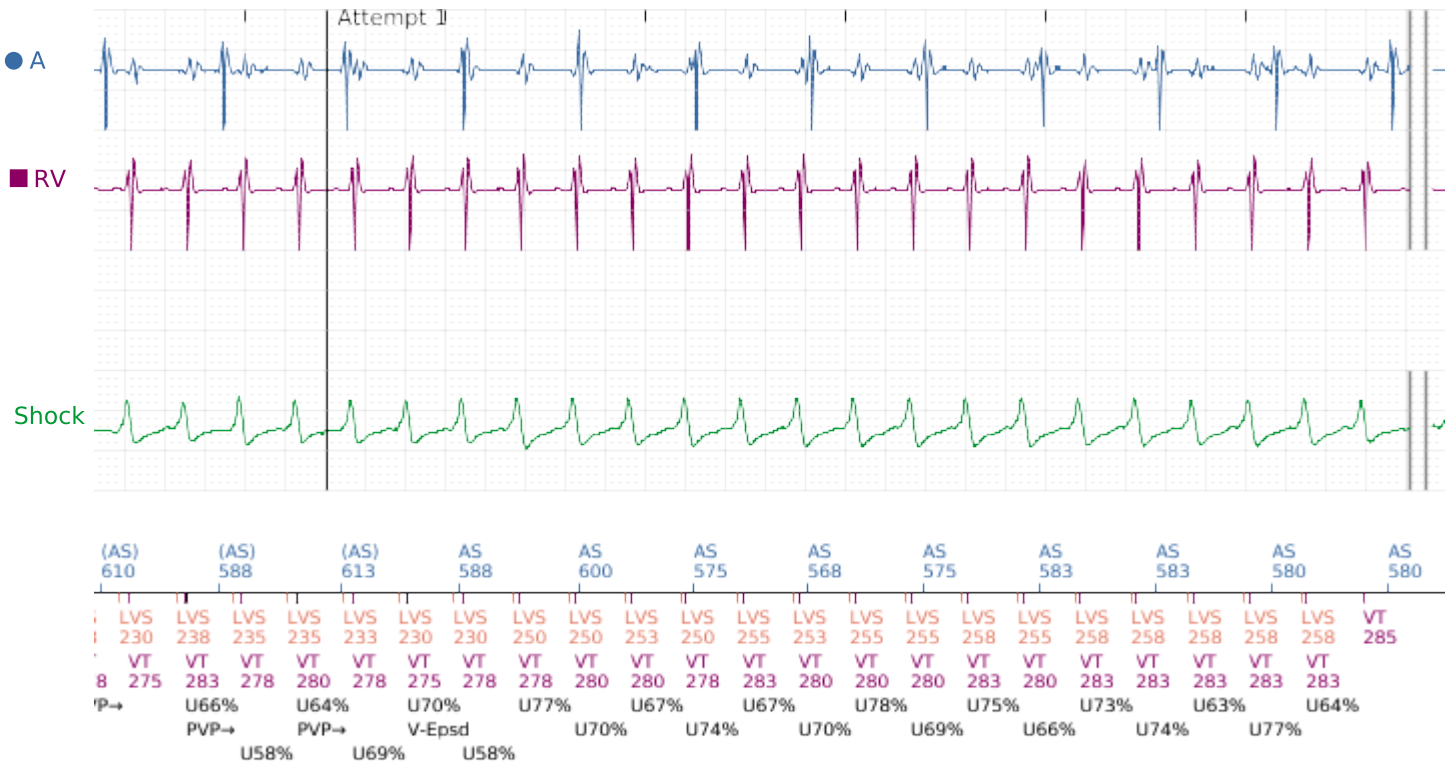



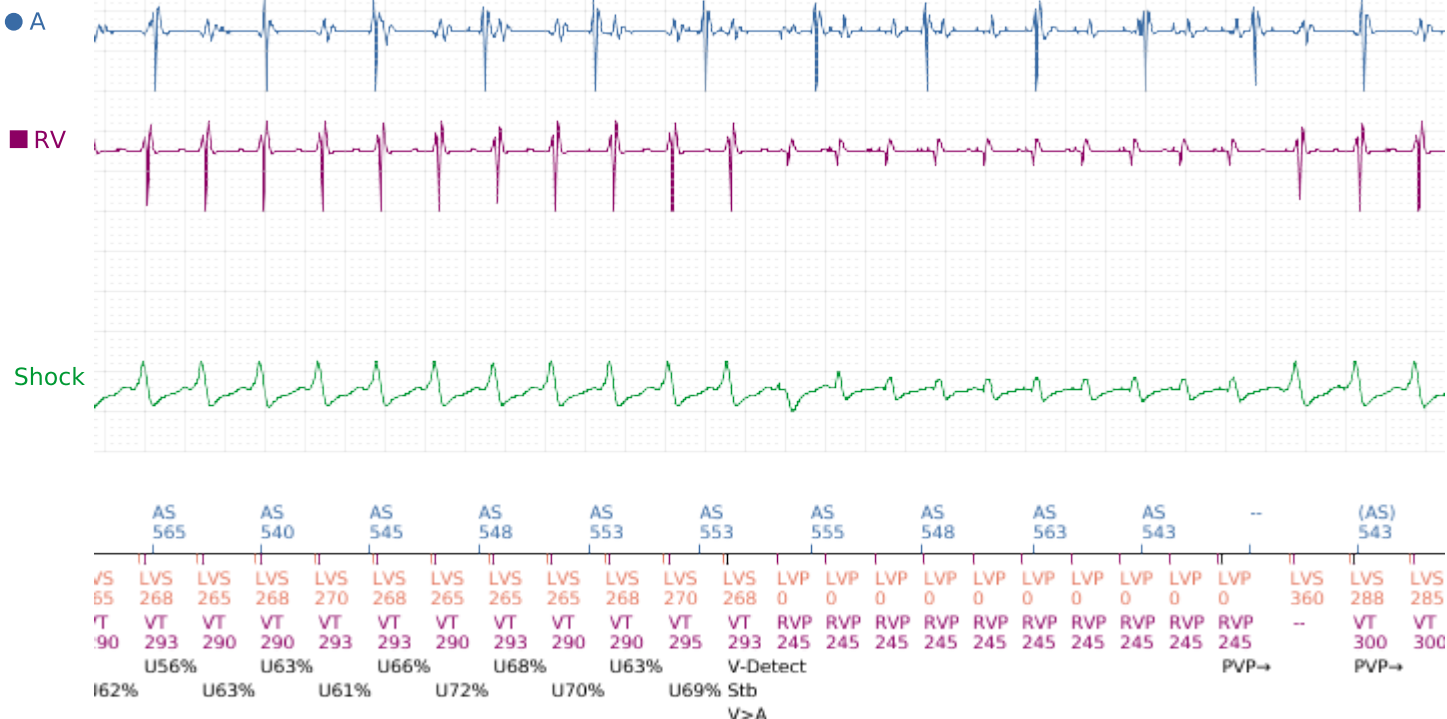






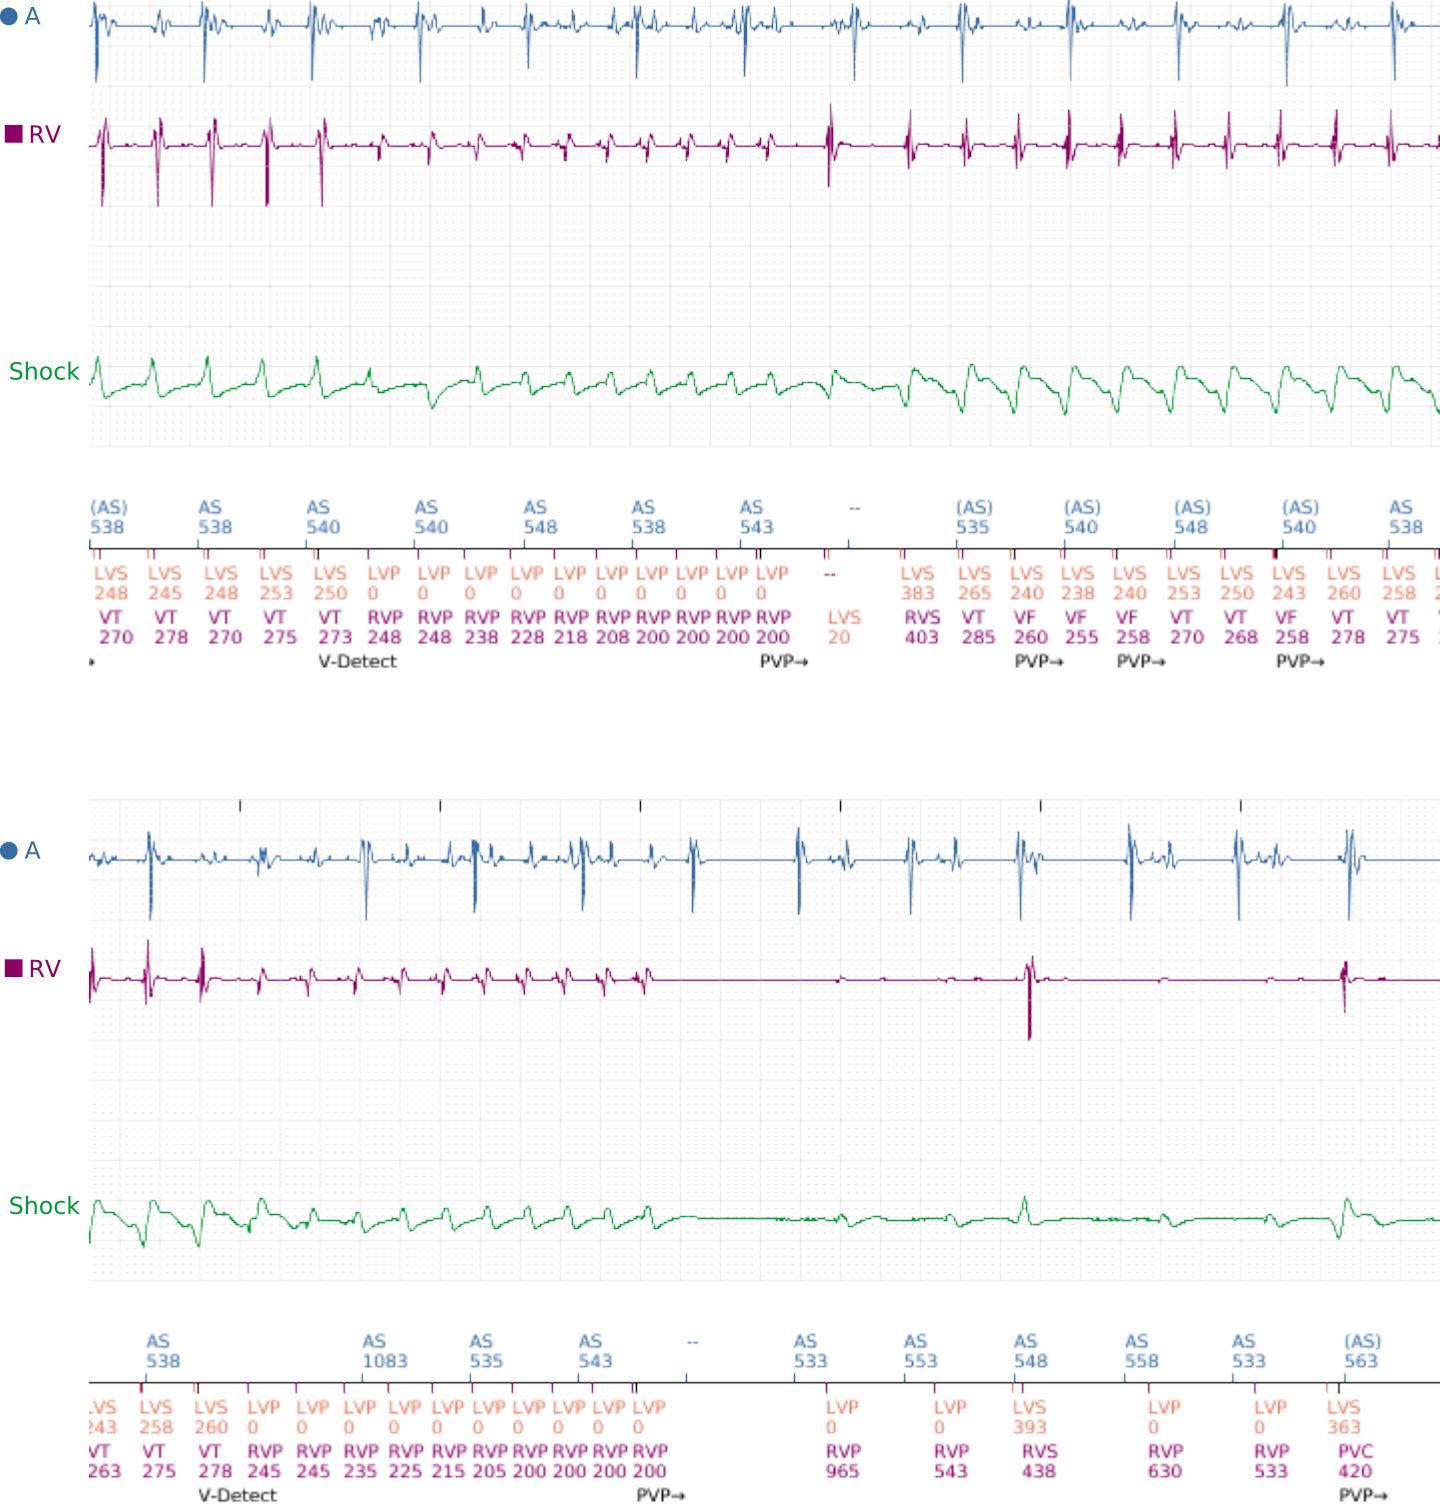

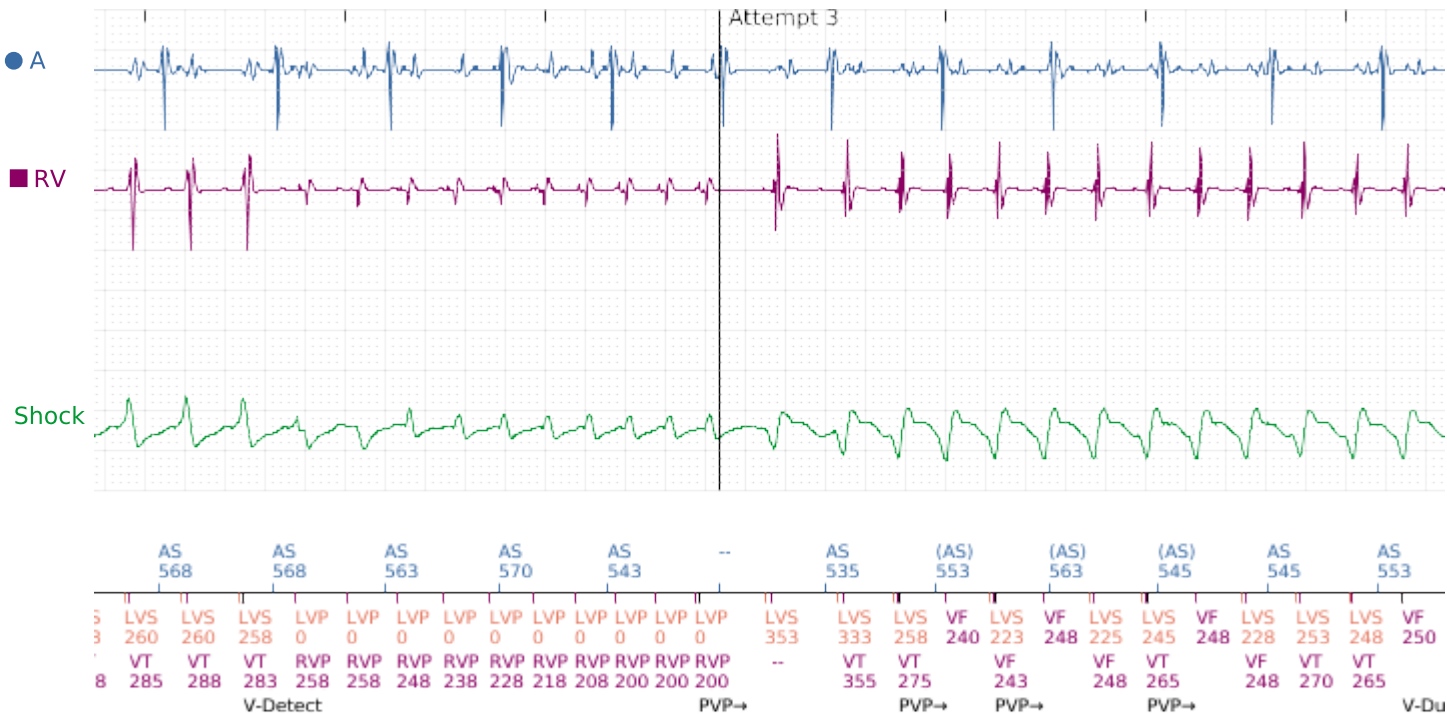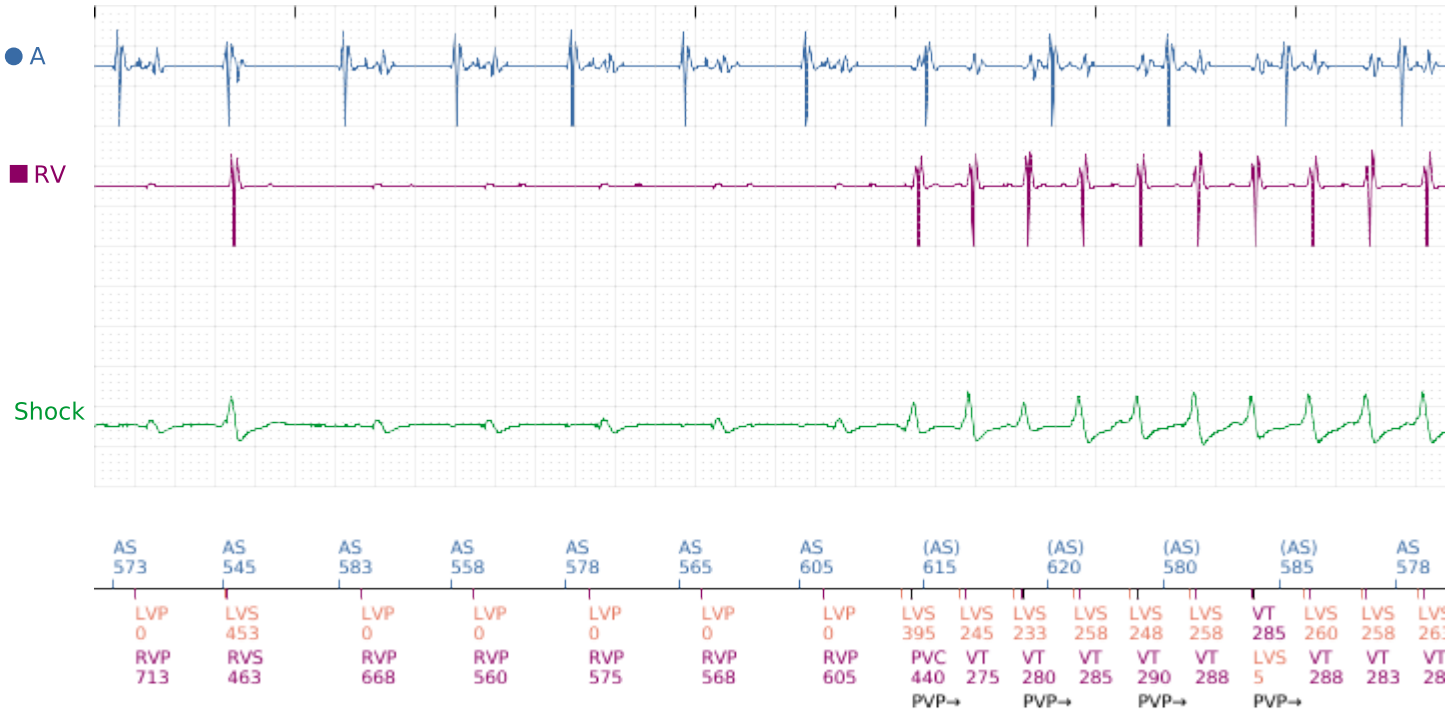

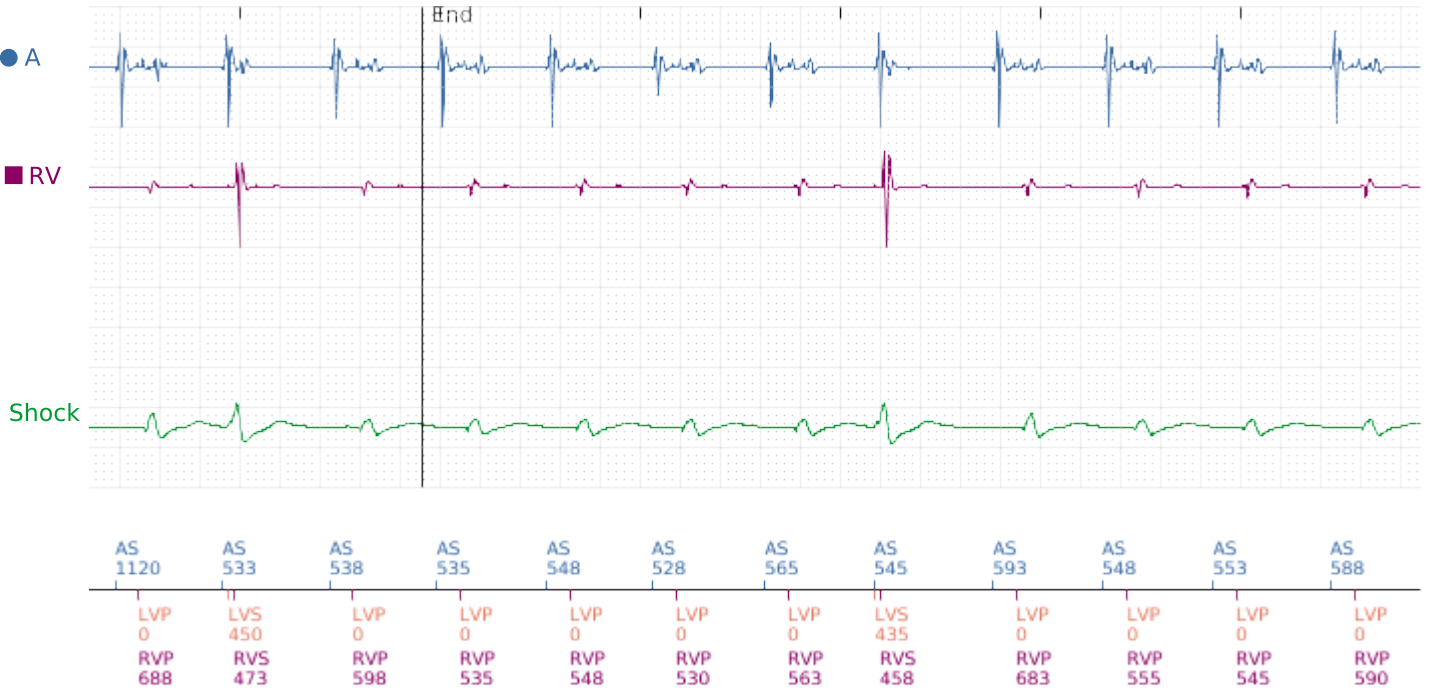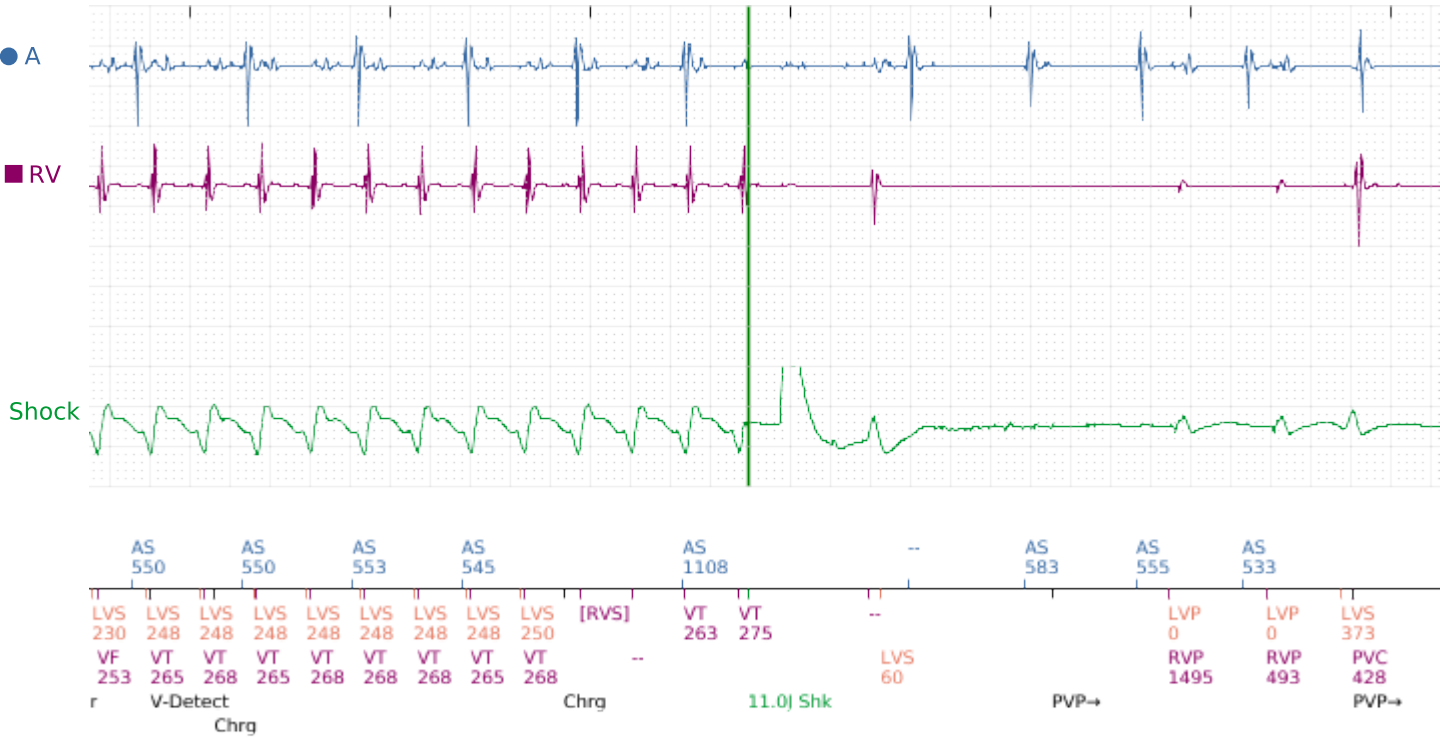

↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

