


LATITUDE™ Patient Management - Event Detail Report		Report Created: 23 Jan 2023
	Date of Birth:	Latest Device Transmission: 05 Apr 2018 02:51 CEST
	Device: INCEPTA CRT-D P163	Last Office Interrogation: 05 Feb 2018
	Clinic:	Implant Date:
	Search Tags:	Patient Group:
	Tachy Mode: Monitor + Therapy	

V-832: 05 Feb 2018 09:31, VT, A Rate: 69 min⁻¹, V Rate: 153 min⁻¹



Detail


VT Event Onset			
Avg A Rate	69 min ⁻¹		
Avg V Rate	153 min ⁻¹		
Detection	Rate Only		
Template	N/R		
At V-Detect		Attempt 1, Burst V ATP	
Avg A Rate	71 min ⁻¹	Elapsed Time	00:00:04
Avg V Rate	152 min ⁻¹	ATP Information	
Rate Zone	VT	Number of Bursts	4
Stability	(13 ms, Off)		
V>A Rate	(True, Off)		
AFib	(False, Off)		
RhythmMatch™	N/R		
SRD Met	(False, Off)		
ATP Timeout	False		
Onset Intvl	(8 ms, Off)		
Onset %	(1 %, Off)		
At V-Detect		Attempt 2, Ramp V ATP	
Avg A Rate	66 min ⁻¹	Elapsed Time	00:00:45
Avg V Rate	154 min ⁻¹	ATP Information	
Rate Zone	VT	Number of Bursts	3
ATP Timeout	False		
At V-Detect		Attempt 3, 11 J V Shock	
Avg A Rate	66 min ⁻¹	Elapsed Time	00:01:19
Avg V Rate	156 min ⁻¹	Shock Information	
Rate Zone	VT	Charge Time	2.3 s
ATP Timeout	False	Lead Impedance	35 Ω
		Lead Polarity	Initial
At V-Detect		Attempt 4, 41 J V Shock	
Avg A Rate	N/R	Elapsed Time	00:01:26
Avg V Rate	274 min ⁻¹	Shock Information	
Rate Zone	VF	Charge Time	11.2 s
Stability	(5 ms, Off)	Lead Impedance	37 Ω
V>A Rate	(True, Off)	Lead Polarity	Initial
AFib	(False, Off)		
SRD Met	(False, Off)		
ATP Timeout	False		
Event Ended		00:02:10	
EGM displayed at 25mm per second			

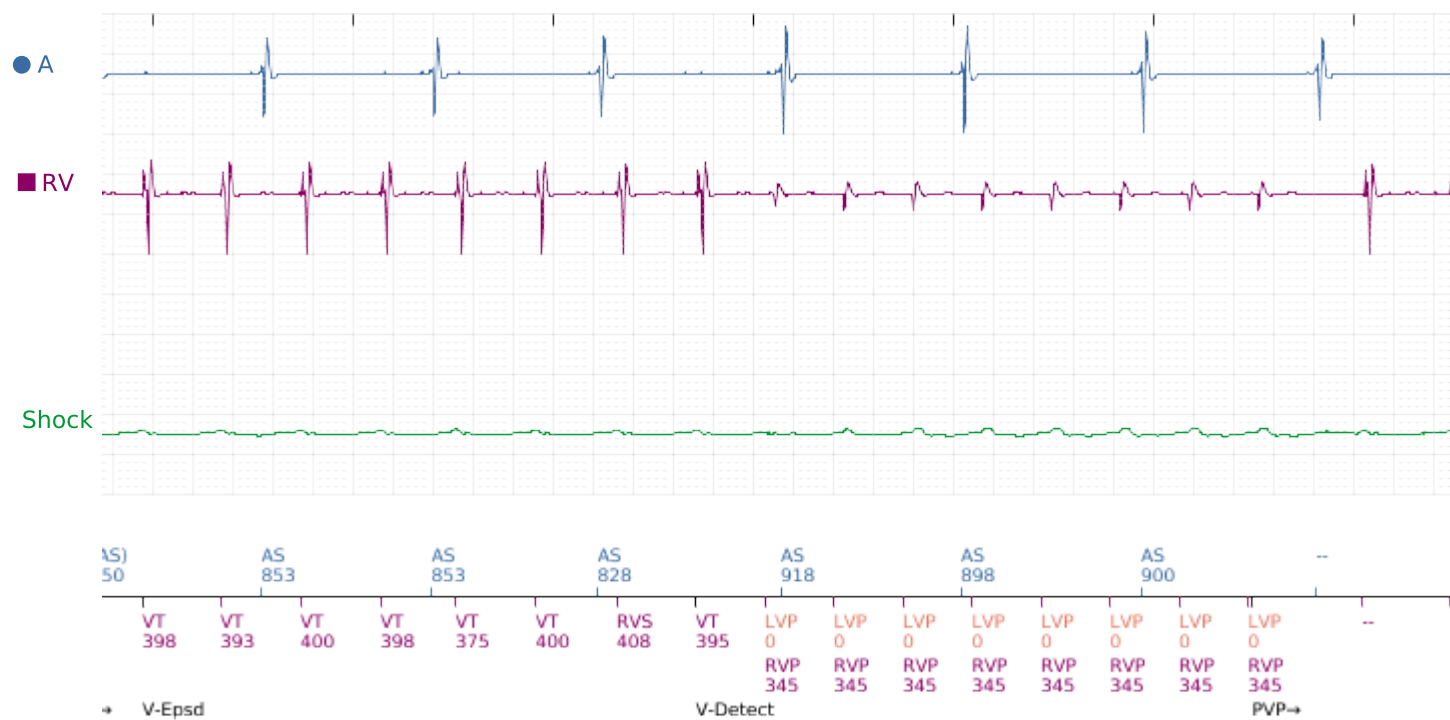








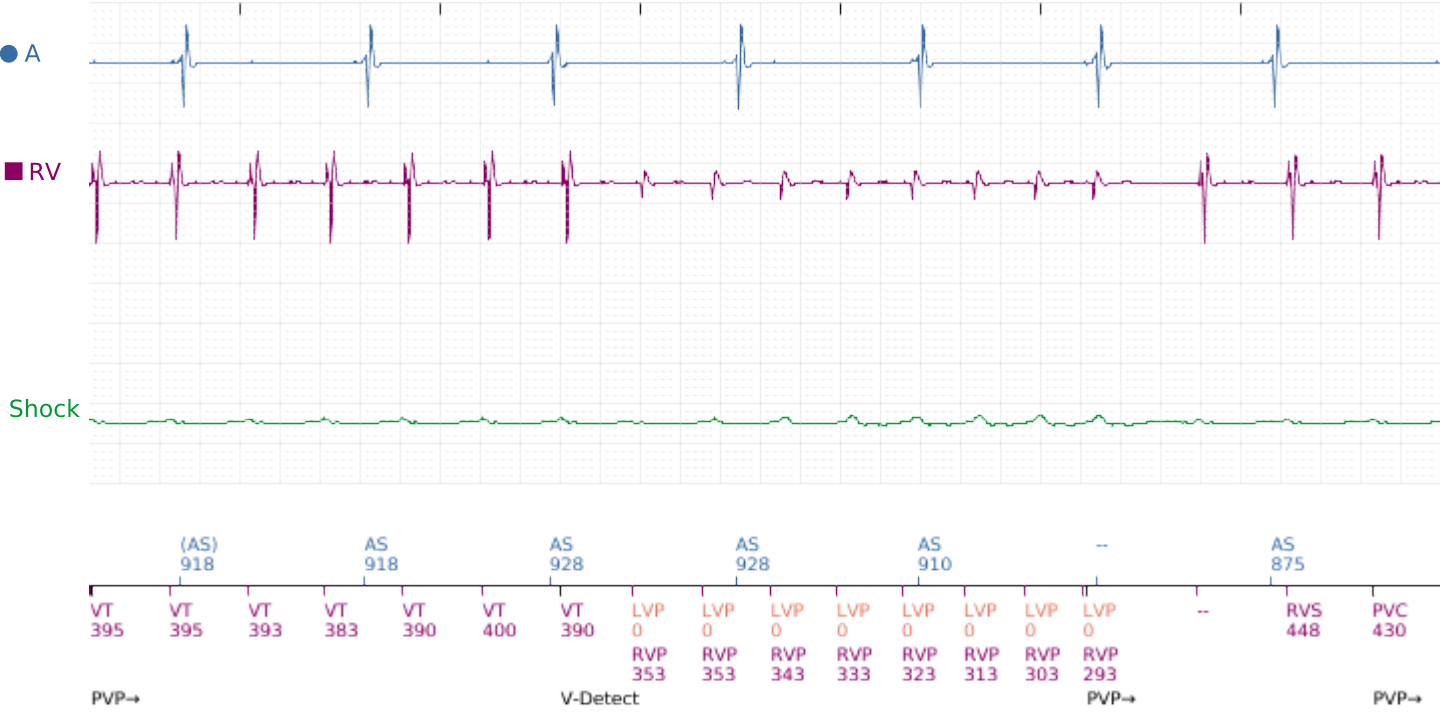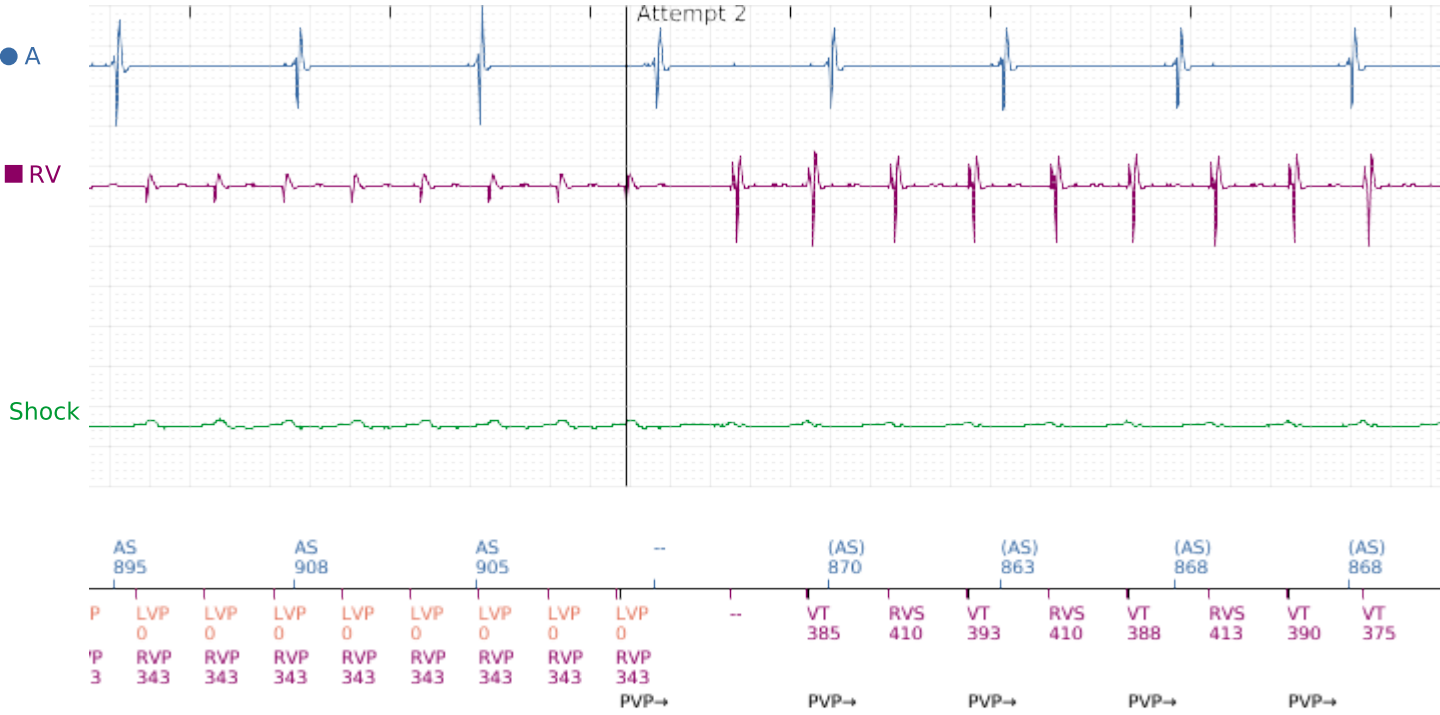

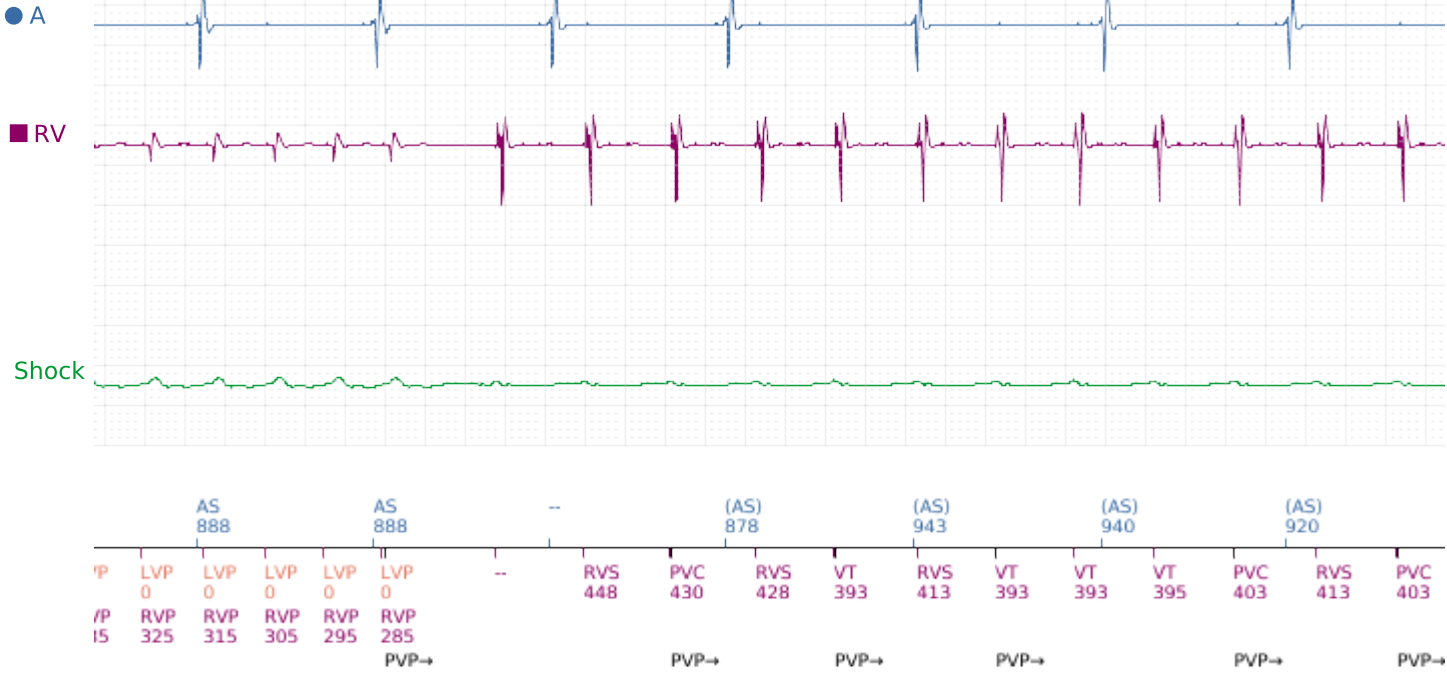



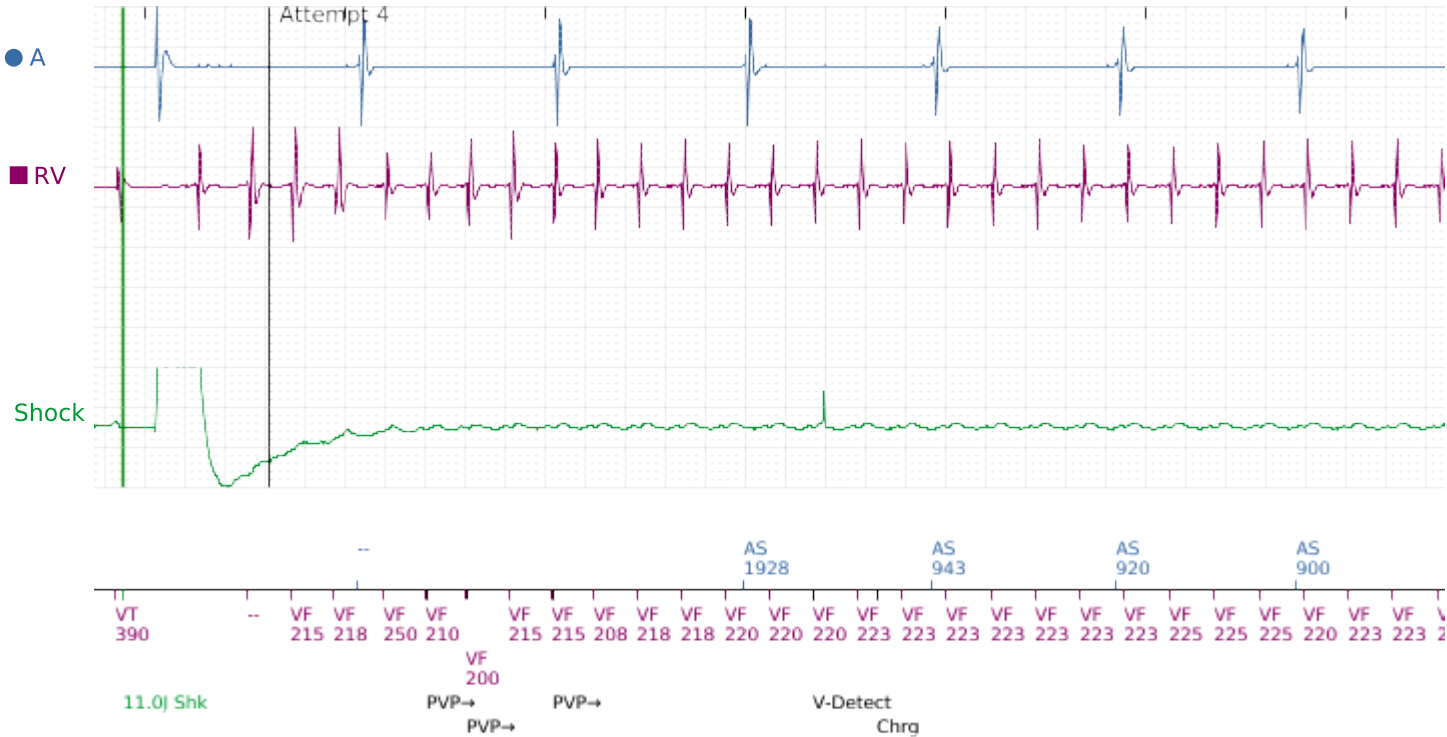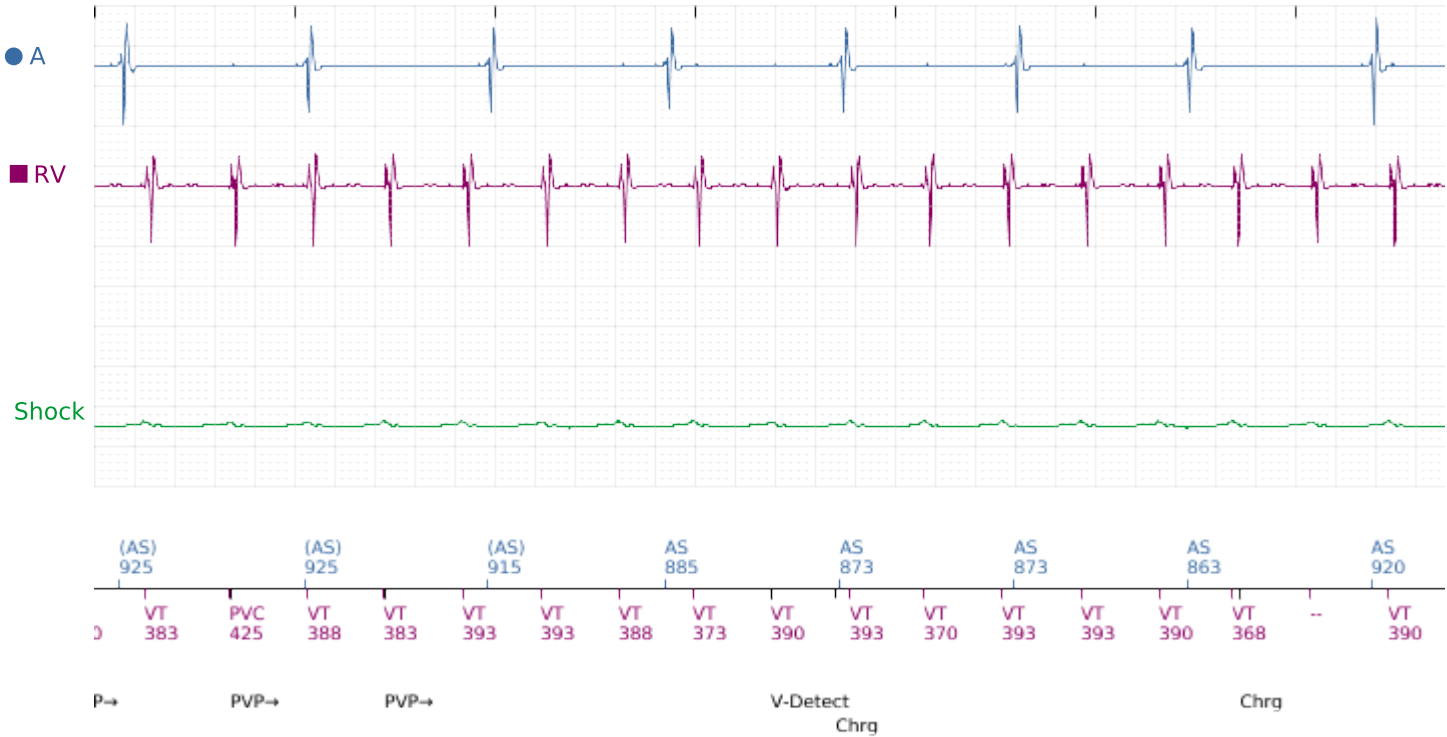

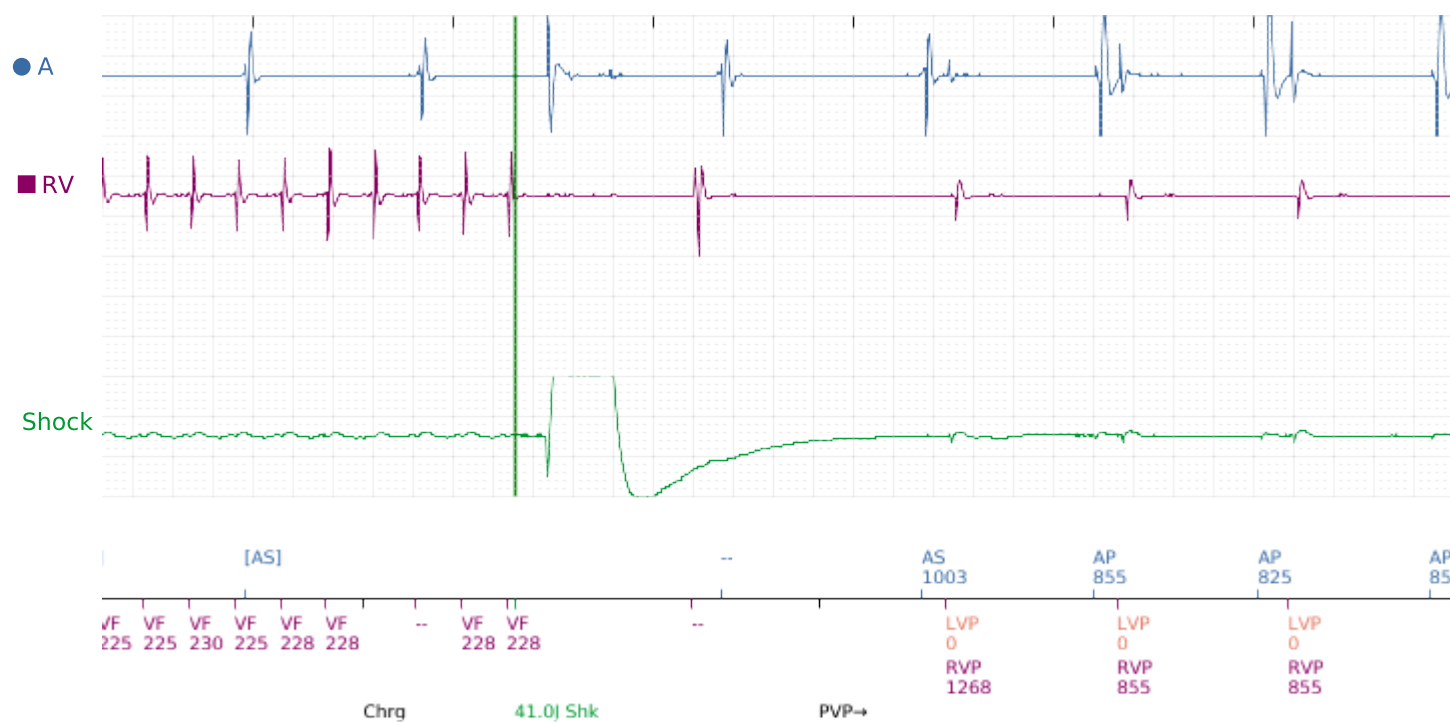



↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	○ A Pace

