

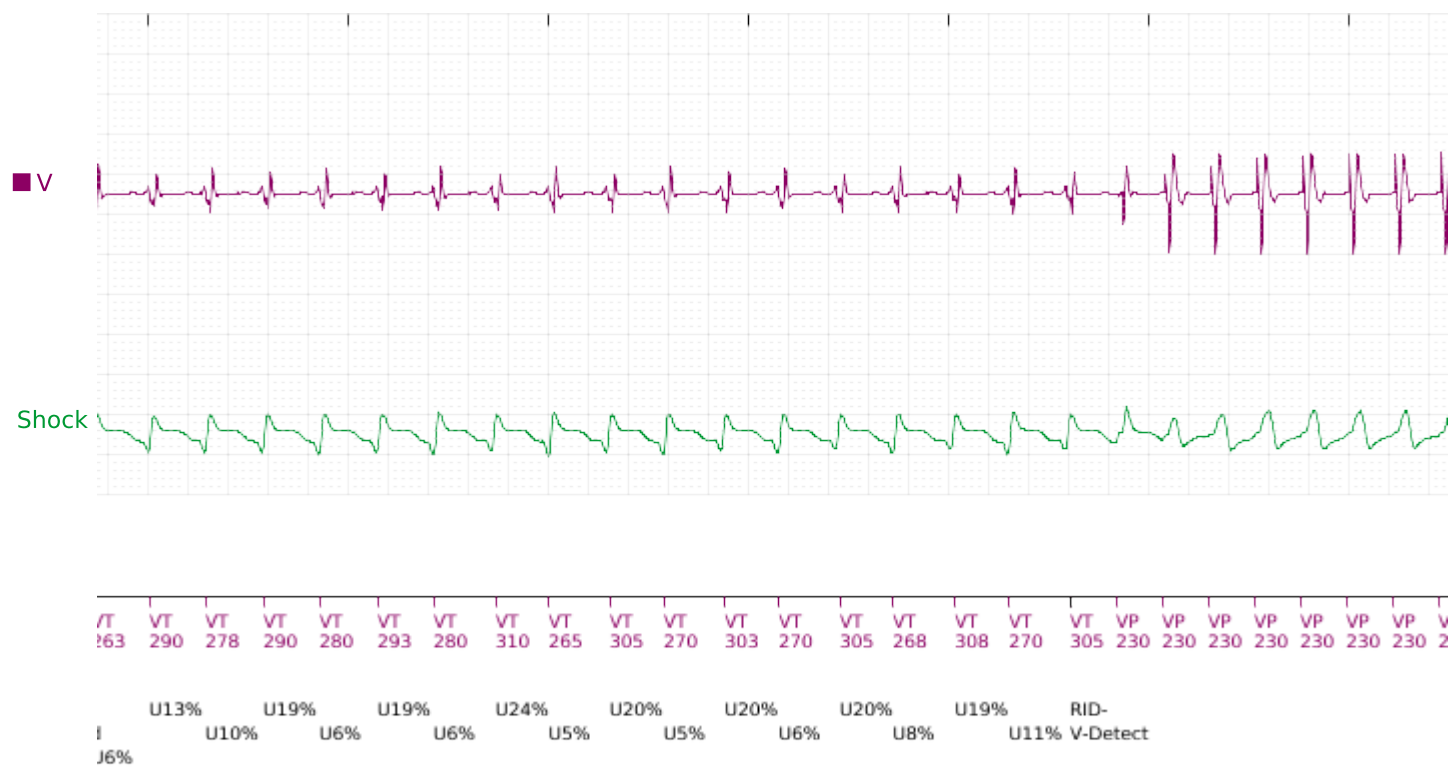



V-3: 20 Jul 2013 11:14, VT, V Rate: 211 min⁻¹



Detail


VT Event Onset			
Avg V Rate	211 min ⁻¹		
Detection	Rhythm ID		
At V-Detect			
Avg V Rate	209 min ⁻¹	Attempt 1, Burst V ATP	
Rate Zone	VT	Elapsed Time	00:00:06
RhythmID Correlated	False	ATP Information	
RhythmMatch™		Number of Bursts	3
SRD Met	False		
ATP Timeout	False		
At V-Detect			
Avg V Rate	211 min ⁻¹	Attempt 2, Ramp V ATP	
Rate Zone	VT	Elapsed Time	00:00:25
ATP Timeout	False	ATP Information	
		Number of Bursts	3
At V-Detect			
Avg V Rate	209 min ⁻¹	Attempt 3, 41 J V Shock	
Rate Zone	VT	Elapsed Time	00:00:44
ATP Timeout	False	Shock Information	
		Charge Time	9.0 s
		Lead Impedance	53 Ω
		Lead Polarity	Initial
Event Ended			00:01:24
EGM displayed at 25mm per second			

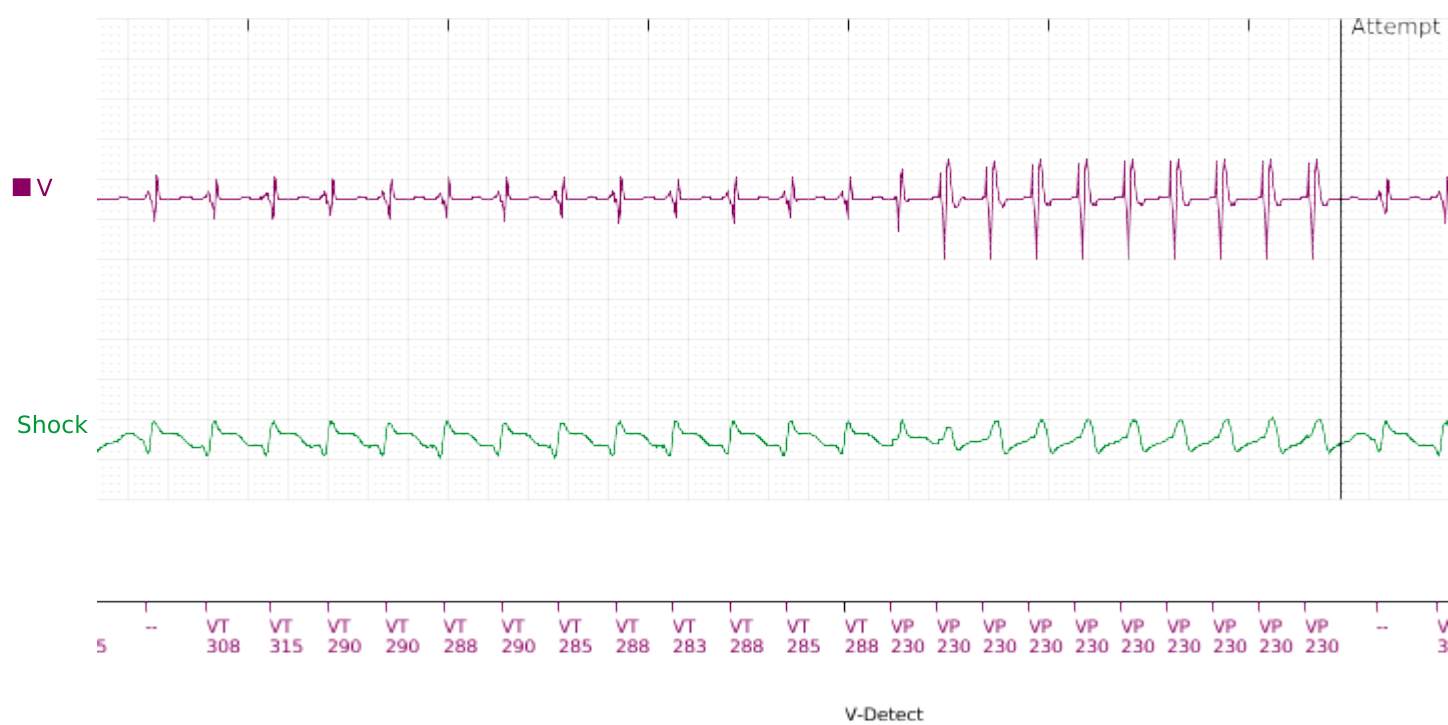


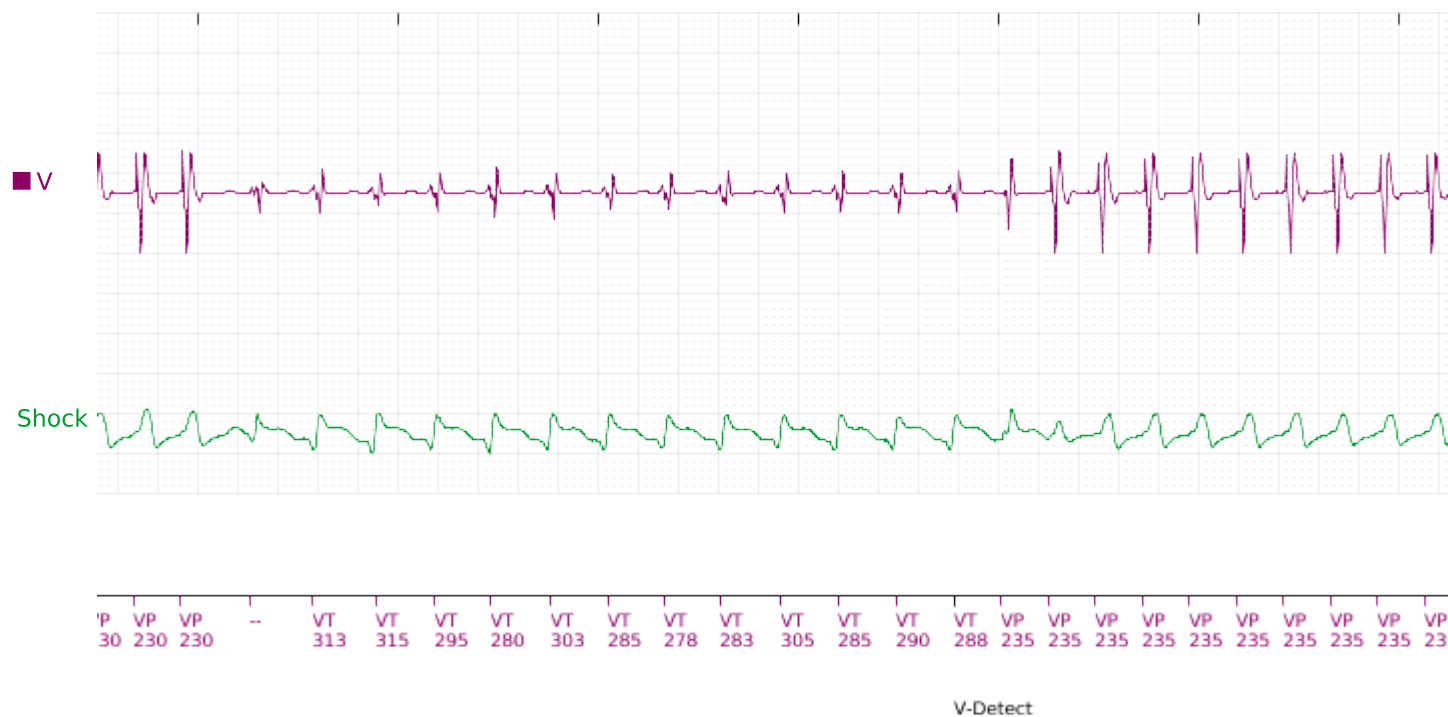

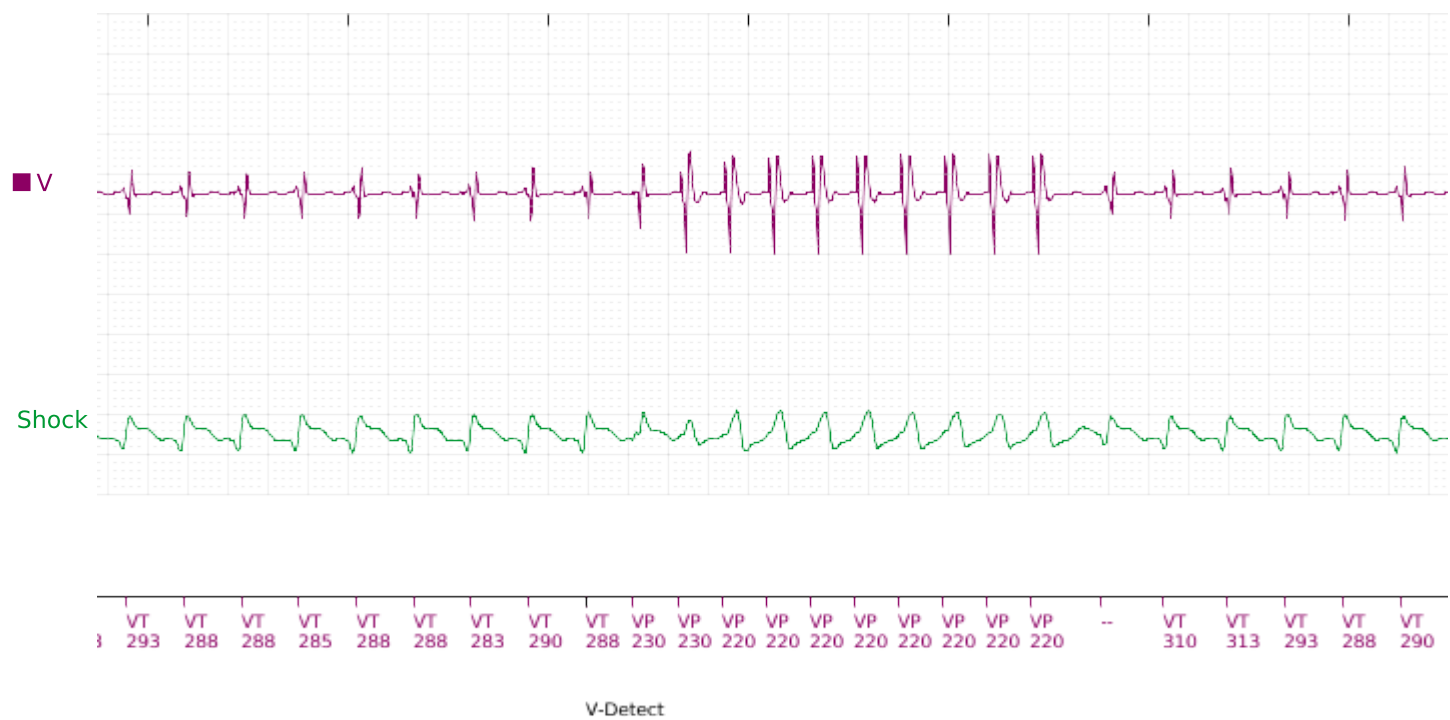

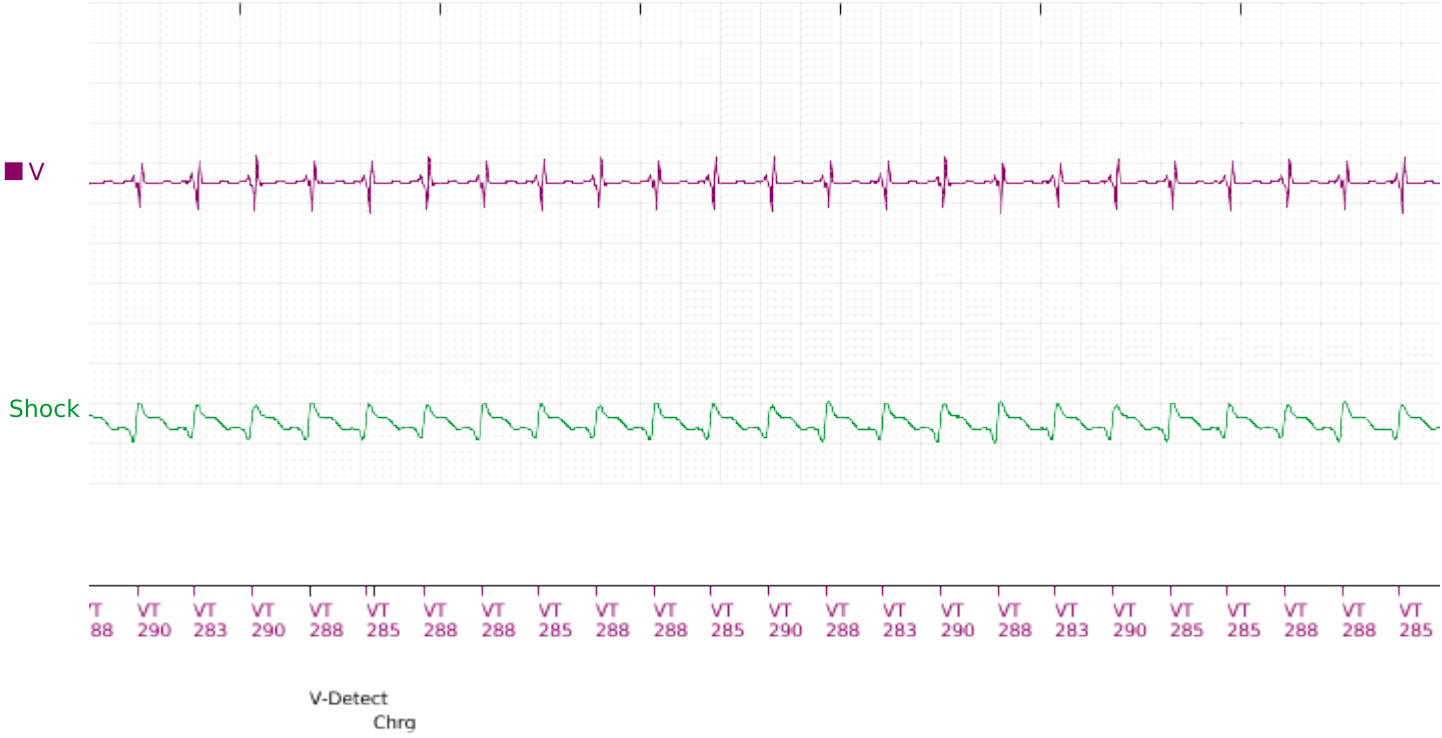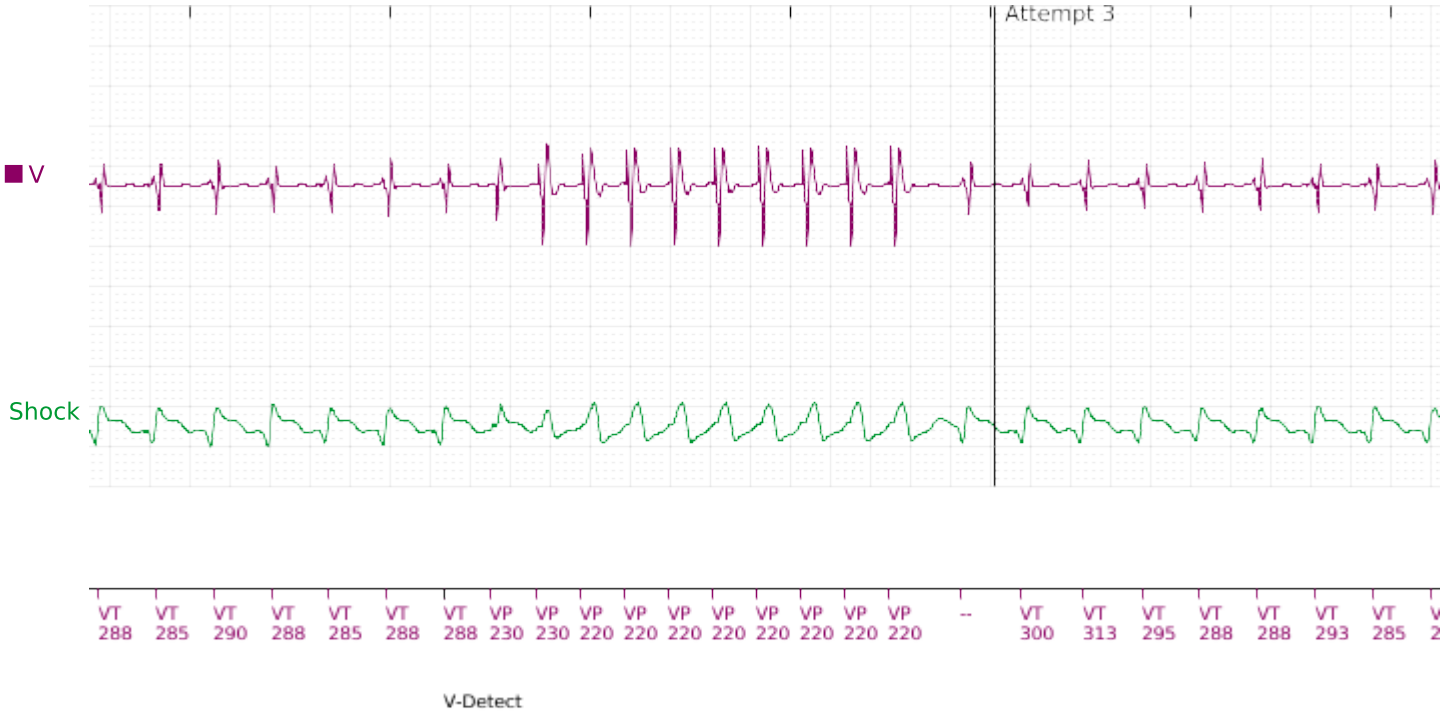

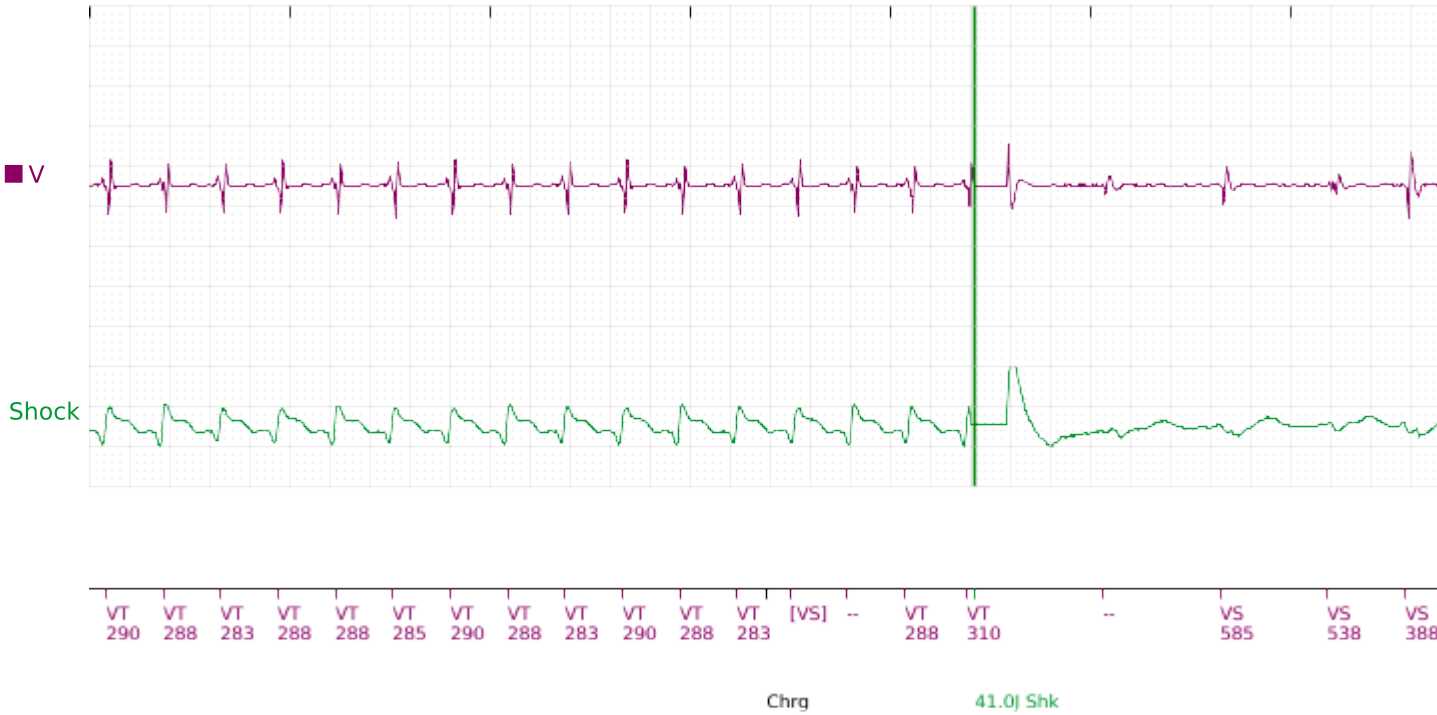

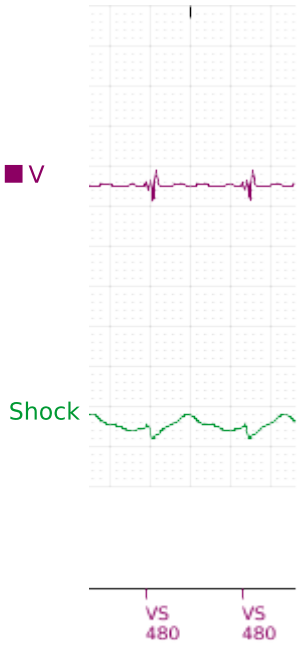

↑ > V Range

↓ < V Range

■ V Sense

□ V Pace

