

LATITUDE™ Patient Management - Event Detail Report		Report Created: 23 Jan 2023
	Date of Birth:	Latest Device Transmission: 20 Dec 2021 02:01 CET
	Device: MOMENTUM X4 CRT-D	Last Office Interrogation: 24 Nov 2021
	Clinic:	Implant Date:
	Search Tags:	Patient Group:
	Tachy Mode: Monitor + Therapy	



V-2: 24 Nov 2021 10:15, VT, A Rate: 82 min⁻¹, V Rate: 209 min⁻¹


Detail



VT Event Onset			
Avg A Rate	82 min ⁻¹		
Avg V Rate	209 min ⁻¹		
Detection	Rhythm ID		
Template	21 Nov 2021 20:55		
RhythmMatch™ Threshold	94 %		
At V-Detect			
Avg A Rate	79 min ⁻¹	Attempt 1, Burst V ATP	
Avg V Rate	204 min ⁻¹	Elapsed Time	00:00:10
Rate Zone	VT	ATP Information	
Stability	4 ms	Number of Bursts	1
V>A Rate	True		
AFib	False		
RhythmID Correlated	False		
RhythmMatch™	64 %		
SRD Met	(False, Off)		
ATP Timeout	False		
Attempt 2, 41 J V Shock			
At V-Detect		Elapsed Time	00:00:16
Avg A Rate	77 min ⁻¹	Shock Information	
Avg V Rate	294 min ⁻¹	Charge Time	9.4 s
Rate Zone	VF	Lead Impedance	38 Ω
ATP Timeout	False	Lead Polarity	Initial
Event Ended			00:00:58
EGM displayed at 25mm per second			

Clinician Signature

Clinician

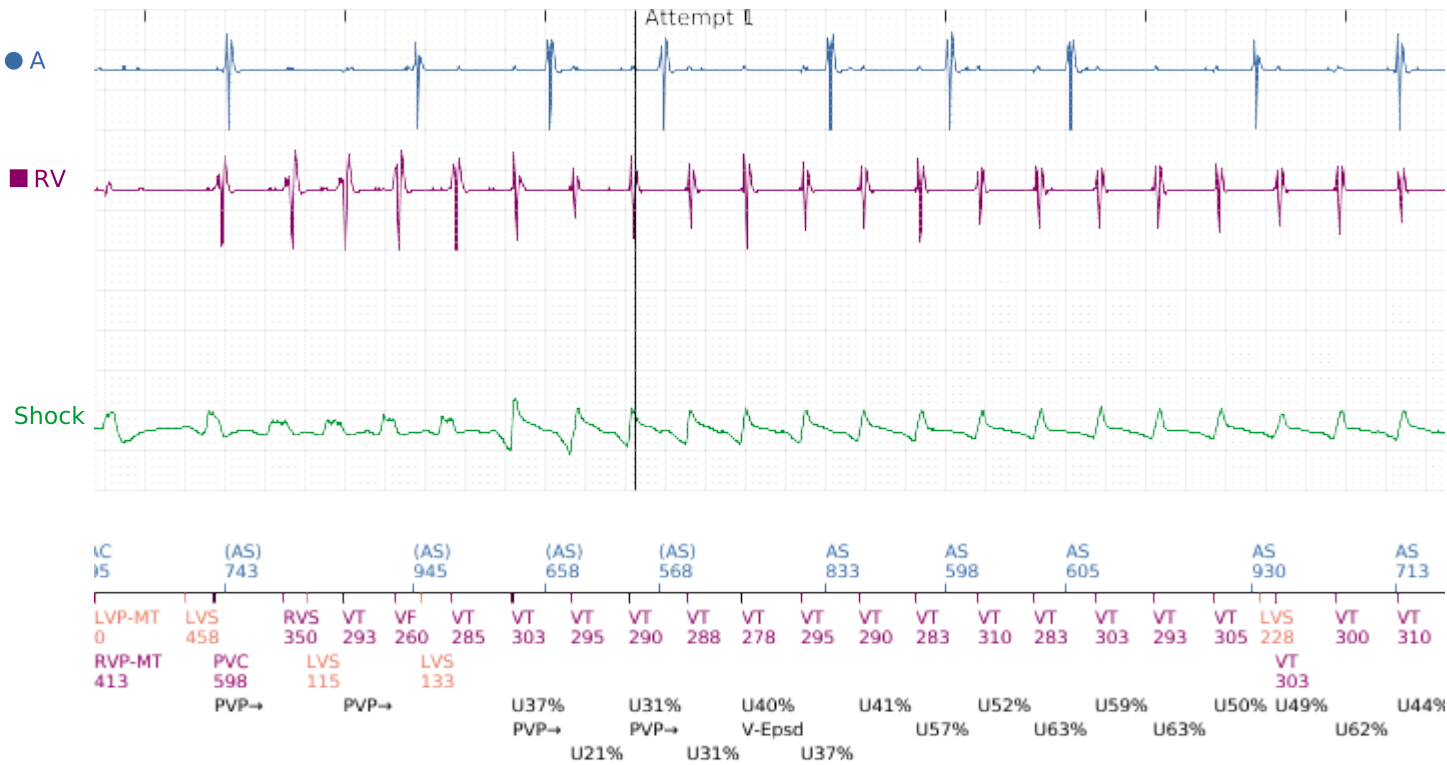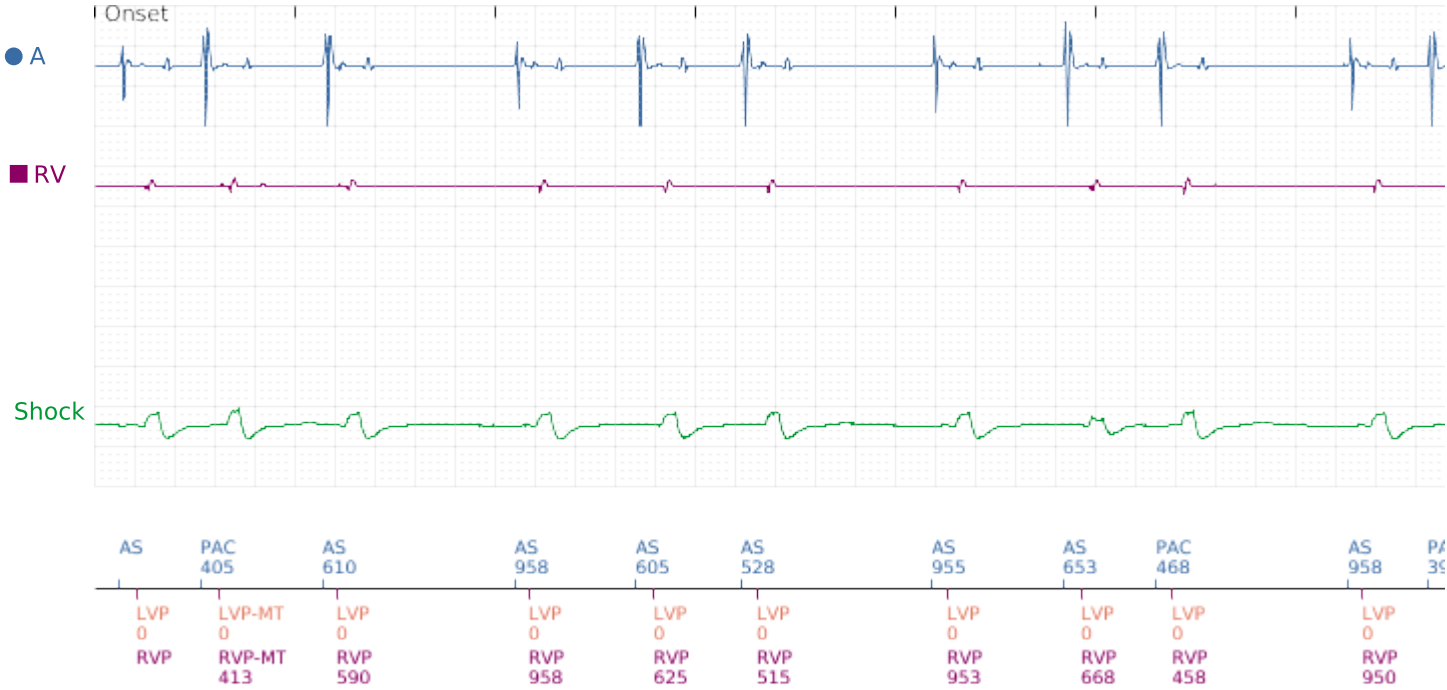

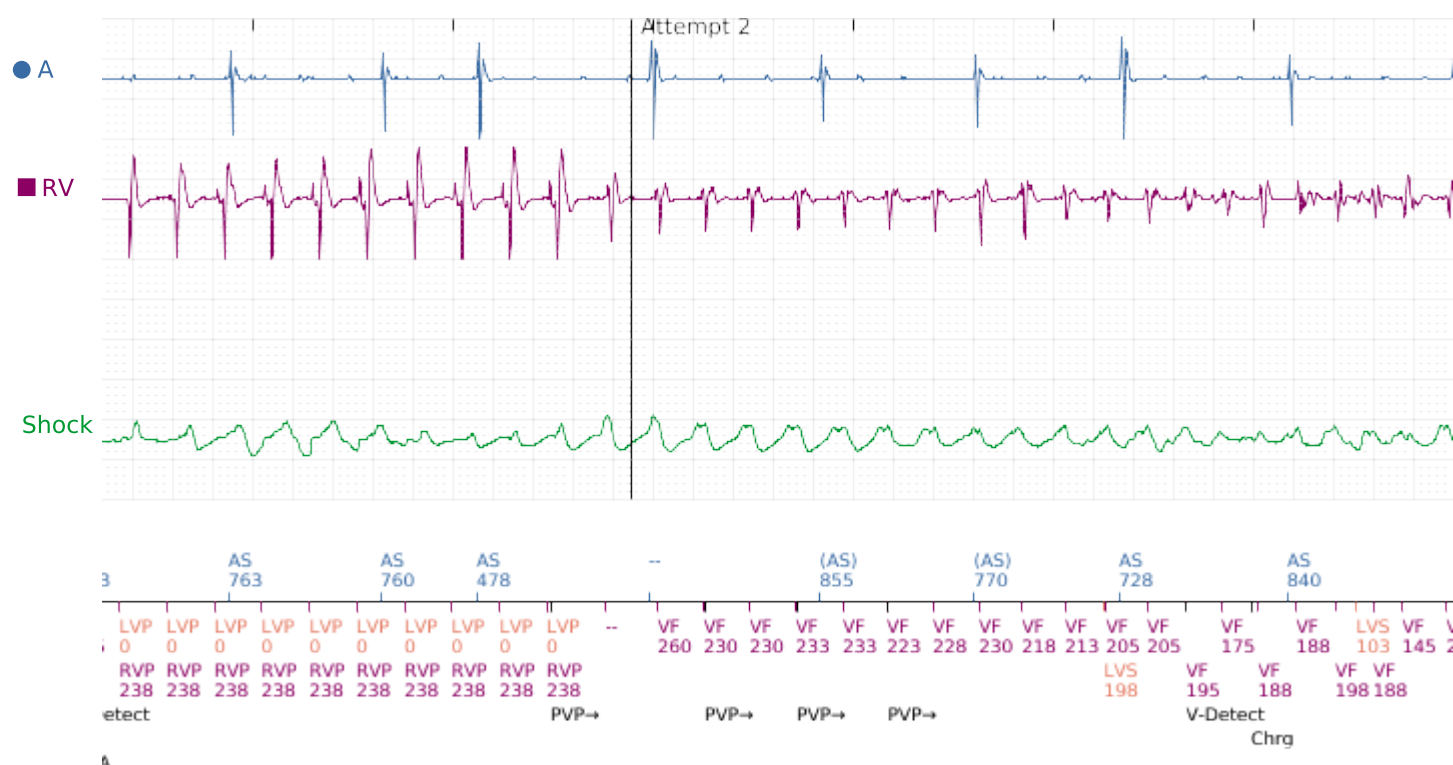

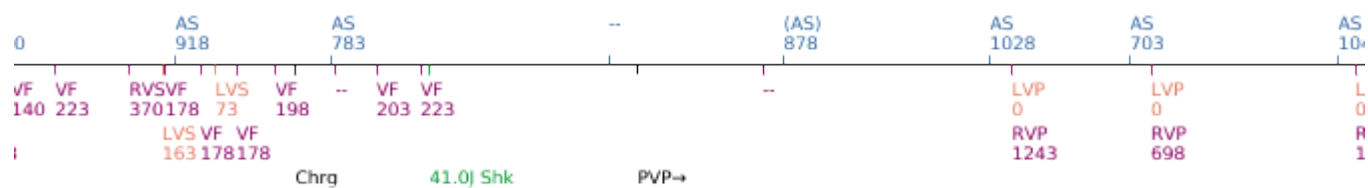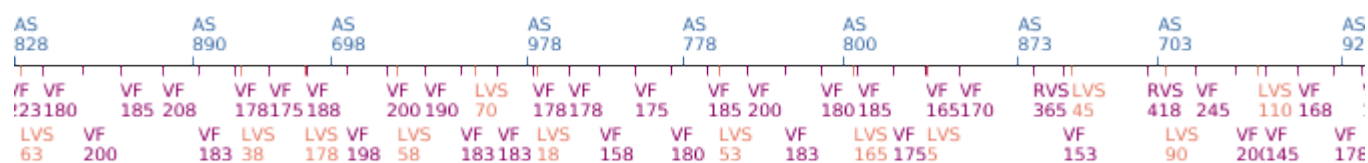



↑ > V Range	↓ < V Range	■ V Sense	□ V Pace
↑ > A Range	↓ < A Range	• A Sense	◦ A Pace

